




Pile Dynamics, Inc.

Transducer 1993

Strain ($\mu\epsilon$)

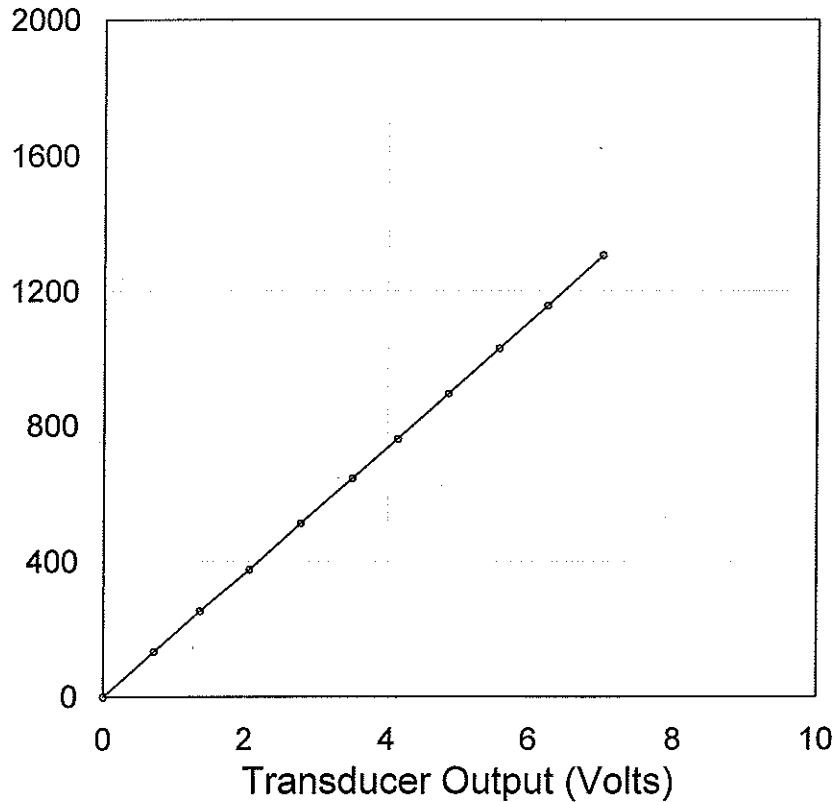

PDA Cal Factor (5.0 V)

93.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
135	0.72
254	1.37
375	2.06
513	2.78
644	3.50
761	4.14
895	4.85
1029	5.56
1158	6.24
1307	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

322.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: Jenny Piscalco
 Calibrated on: 28-Mar-2013

Smart Sensor? Yes No Smart Chip

Programmed by: JP Date: 3-28-13 CRC value E85F