




Pile Dynamics, Inc.

Pile Dynamics, Inc. Transducer K462

Strain ($\mu\epsilon$)

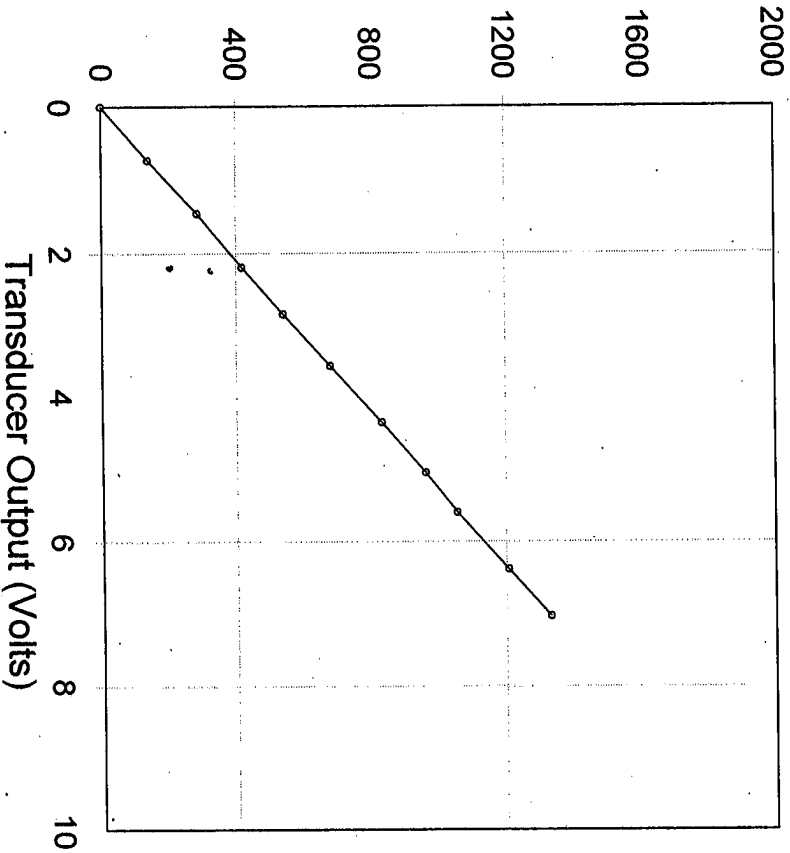

PDA Cal Factor (5.0 V)

94.3 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
139	0.73
284	1.45
416	2.19
539	2.85
676	3.57
830	4.36
960	5.07
1052	5.60
1207	6.38
1331	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

327.4 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: Kay Tsi
Calibrated on: 05-May-2014

Smart Sensor? Yes No Smart Chip

Programmed by: KT Date: 5-5-14 CRC value 10F4