


Certificate of Calibration

Pile Dynamics, Inc.

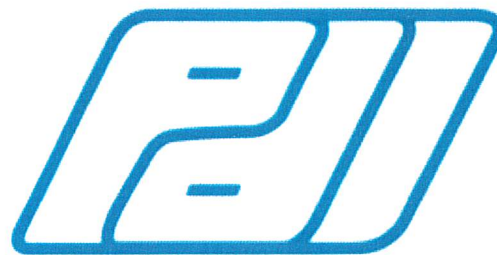

Calibrated by Pile Dynamics, Inc.

Serial No: LW550196 Temperature: 24.5 °C
 Model: PIT ACC Humidity: 44%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
9.8 g's/volt
 R²: 0.999984 [Chip programmed]

Ref Acc 1: LW547722! Cal on: 21Oct2025
 10 g's/volt
 Ref Acc 2: LW547723! Cal on: 21Oct2025
 10 g's/volt

Operator: William Johnson


Signed

Calibration valid 2 years

APR 16 2026

From: _____

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

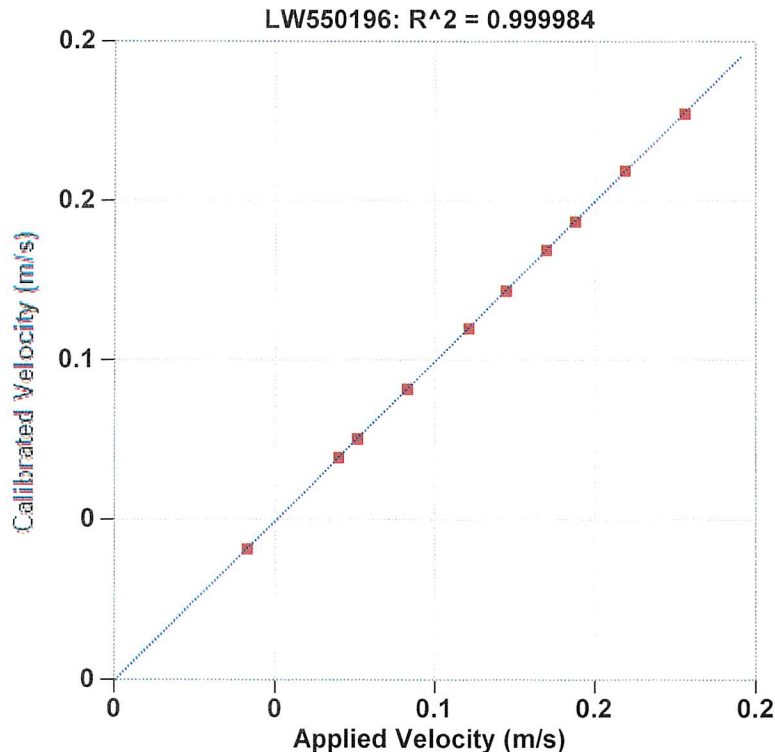

Reference Velocity	S/N LW550196 Velocity
m/s	m/s
0.041	0.041
0.070	0.070
0.076	0.076
0.091	0.091
0.110	0.110
0.122	0.122
0.135	0.135
0.144	0.144
0.159	0.160
0.178	0.178
Maximum Acceleration: 20 g's	