

Certificate of Calibration

Pile Dynamics, Inc.



Calibrated by Pile Dynamics, Inc.

Serial No: LW550240 Temperature: 21.8 °C

Model: PIT ACC Humidity: 23%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

9.7 g's/volt

R²: 0.999993 [Chip programmed]

Ref Acc 1: LW547723! Cal on: 21Oct2025
10 g's/volt

Ref Acc 2: LW547722! Cal on: 21Oct2025
10 g's/volt

Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

APR 16 2026

From: _____

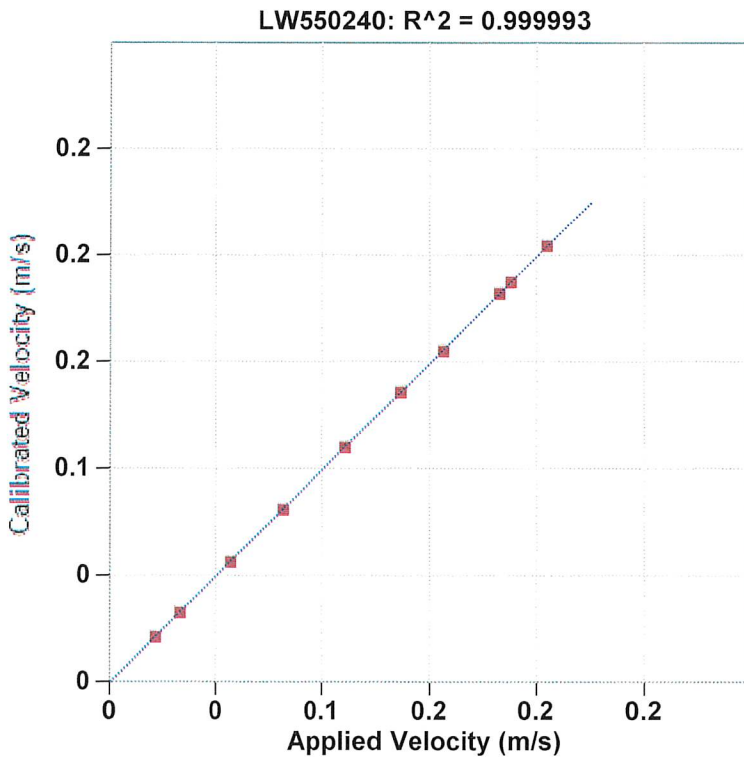

Reference Velocity	S/N LW550240 Velocity
m/s	m/s
0.022	0.021
0.033	0.033
0.057	0.057
0.081	0.081
0.111	0.111
0.136	0.137
0.156	0.156
0.183	0.183
0.188	0.188
0.205	0.205

Maximum Acceleration: 25 g's