

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15271 Temperature: 22.6 °C
 Model: KICHER PR Humidity: 29%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

401.6 mv/5000g
 (80.3 μ v/g)
 R²: 0.999909 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: MAY 19 2026

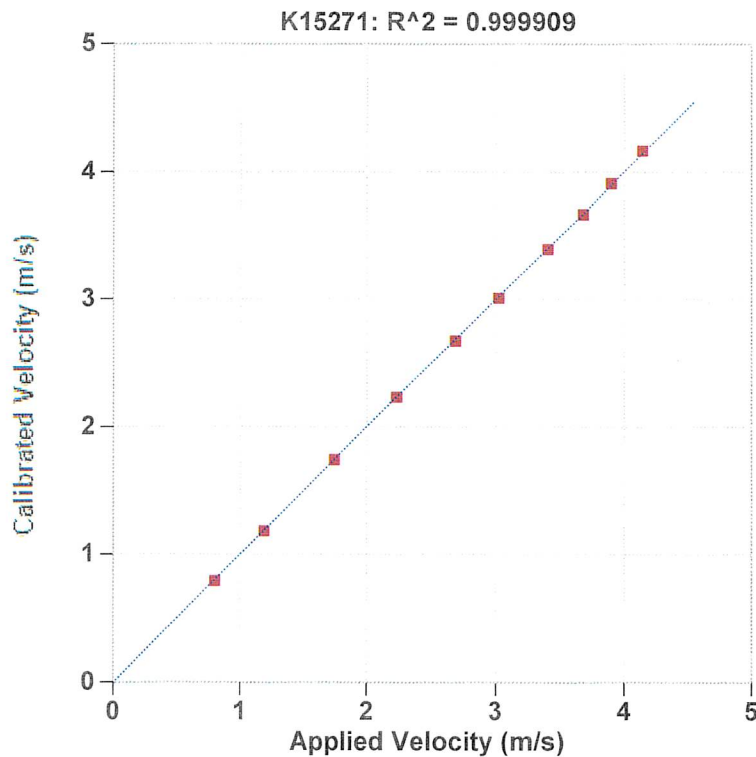

Reference Velocity	S/N K15271 Velocity
m/s	m/s
0.810	0.798
1.193	1.187
1.749	1.746
2.236	2.237
2.689	2.679
3.029	3.013
3.400	3.395
3.671	3.667
3.900	3.912
4.149	4.169

Maximum Acceleration: 884 g's