

Certificate of Calibration

Pile Dynamics, Inc.



Calibrated by Pile Dynamics, Inc.

Serial No: K15279 Temperature: 22.6 °C
 Model: KICHER PR Humidity: 29%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

437.4 mv/5000g
 (87.5 μ v/g)
 R²: 0.999907 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: MAY 19 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

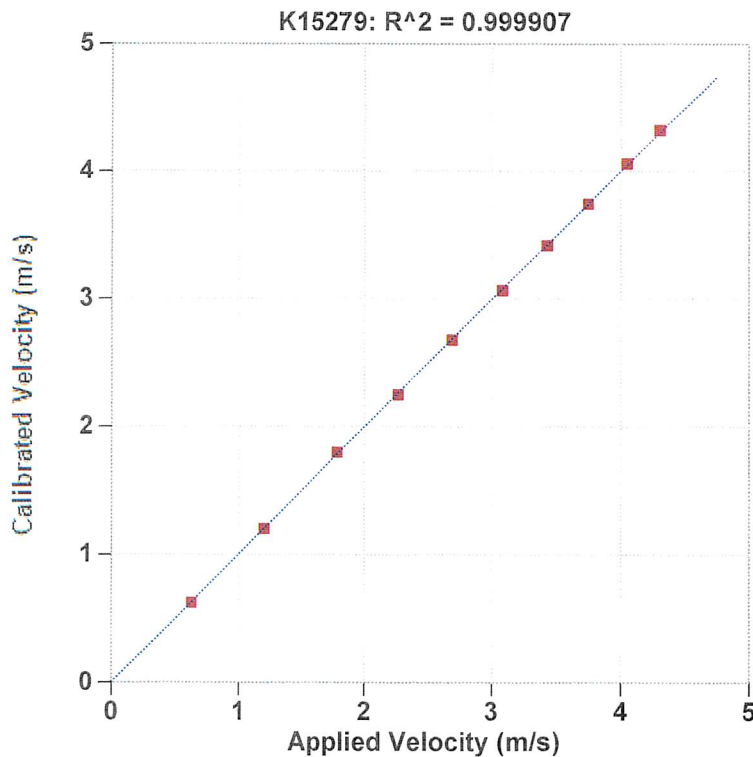

Reference Velocity	S/N K15279 Velocity
m/s	m/s
0.630	0.624
1.208	1.205
1.792	1.806
2.271	2.258
2.694	2.686
3.088	3.073
3.432	3.422
3.750	3.749
4.055	4.065
4.306	4.325

Maximum Acceleration: 920 g's