



Pile Dynamics, Inc.


Pile Dynamics, Inc.

Transducer L031

Strain ($\mu\epsilon$)

PDA Cal Factor (5.0 V)

92.7 $\mu\epsilon/V$

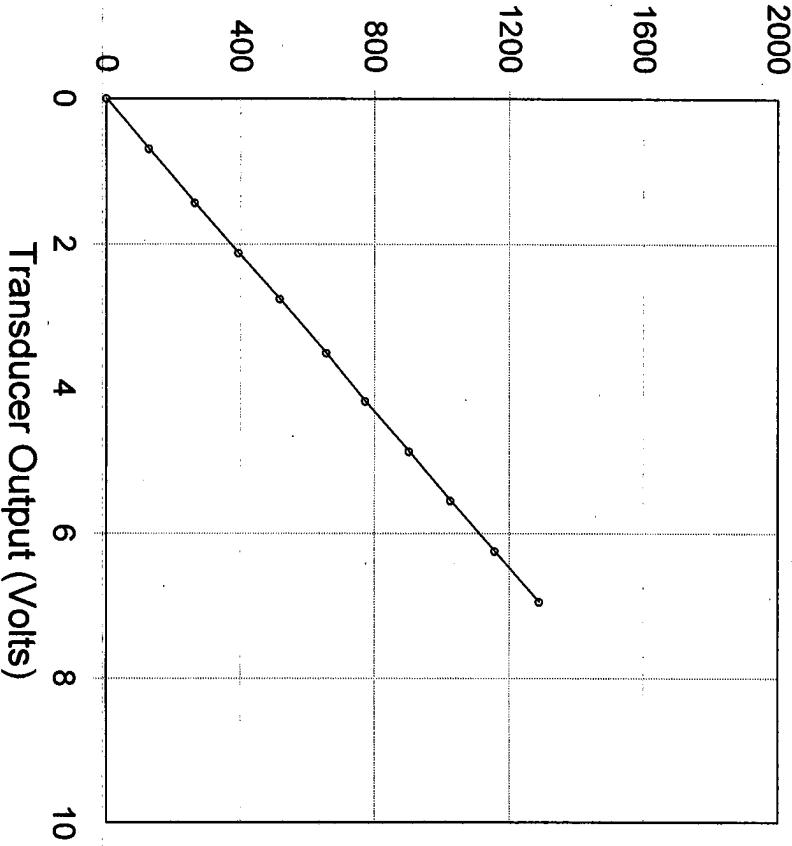

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
126	0.69
264	1.43
392	2.12
516	2.76
655	3.51
772	4.18
902	4.88
1026	5.55
1157	6.24
1288	6.94

Shunt (60.4 K Ω) 2.5 V
 General Factor 321.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Strain-Transducer-Calibrator-System 2014-Version-1-5

Calibrated on: 26-Aug-2014

Smart Sensor? Yes No Smart Chip

Programmed by:

Date: 8-26-14 CRC value 609c