




Pile Dynamics, Inc.

# Pile Dynamics, Inc. Transducer L033

Strain ( $\mu\epsilon$ )

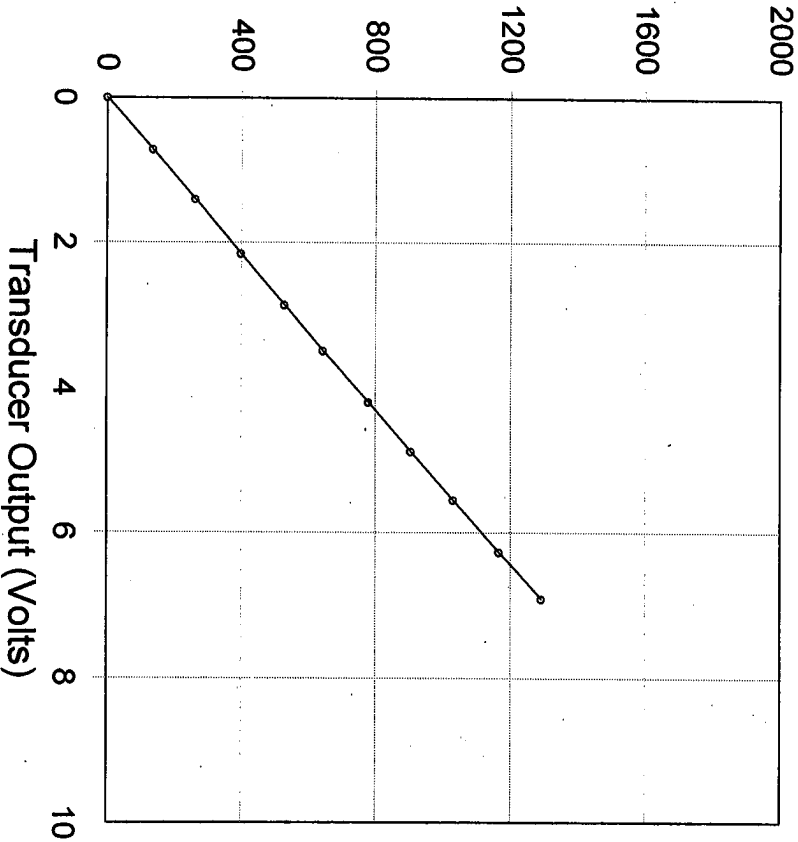

PDA Cal Factor (5.0 V)

93.0 $\mu\epsilon$ /V

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
136	0.72
260	1.41
397	2.15
527	2.85
642	3.48
778	4.19
904	4.88
1030	5.55
1165	6.27
1291	6.92

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

323.1 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Calibrated by:

*W. Stahl*

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated on:

21-Aug-2014

Smart Sensor?  Yes  No Smart Chip

Programmed by:

*W*

Date: 8-21-14

CRC value

*A0E3*