



Pile Dynamics, Inc.

Pile Dynamics, Inc.


Transducer

L034

Strain ($\mu\epsilon$)

PDA Cal Factor (5.0 V)

93.2 $\mu\epsilon$ /V

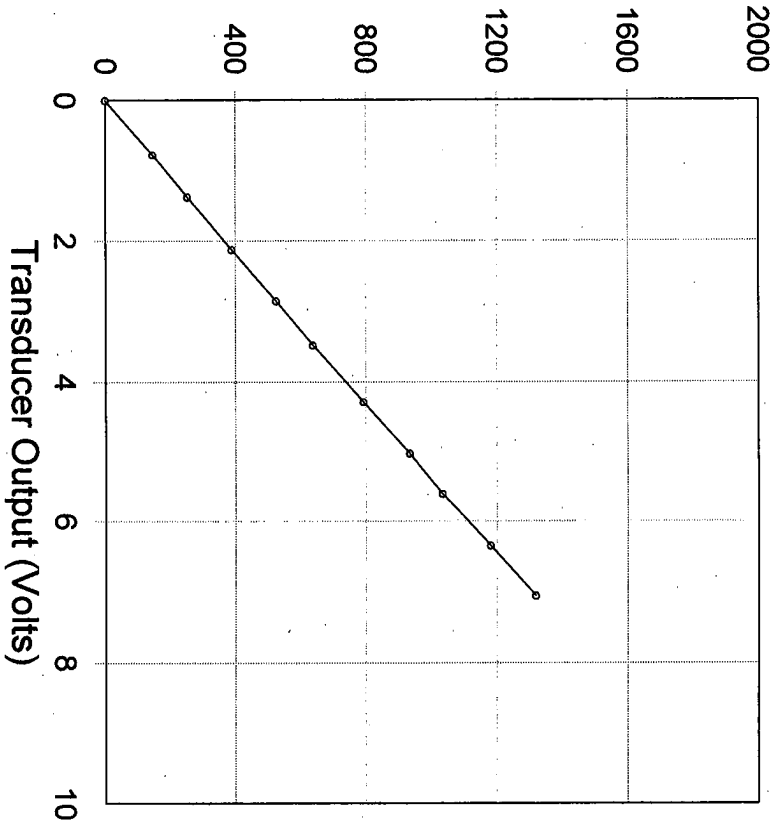

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
147	0.78
252	1.38
389	2.12
525	2.84
638	3.47
793	4.28
933	5.02
1034	5.60
1182	6.34
1319	7.05

Shunt (60.4 K Ω) 2.5 V
 General Factor 323.7 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Calibrated by:

Thack

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated on:

22-Sep-2014

Smart Sensor? Yes No Smart Chip

Programmed by:

LD

Date:

9-23-14

CRC value

3302