


Pile Dynamics, Inc.

# Pile Dynamics, Inc. Transducer L043

Strain ( $\mu\epsilon$ )

PDA Cal Factor (5.0 V)

93.2  $\mu\epsilon/V$

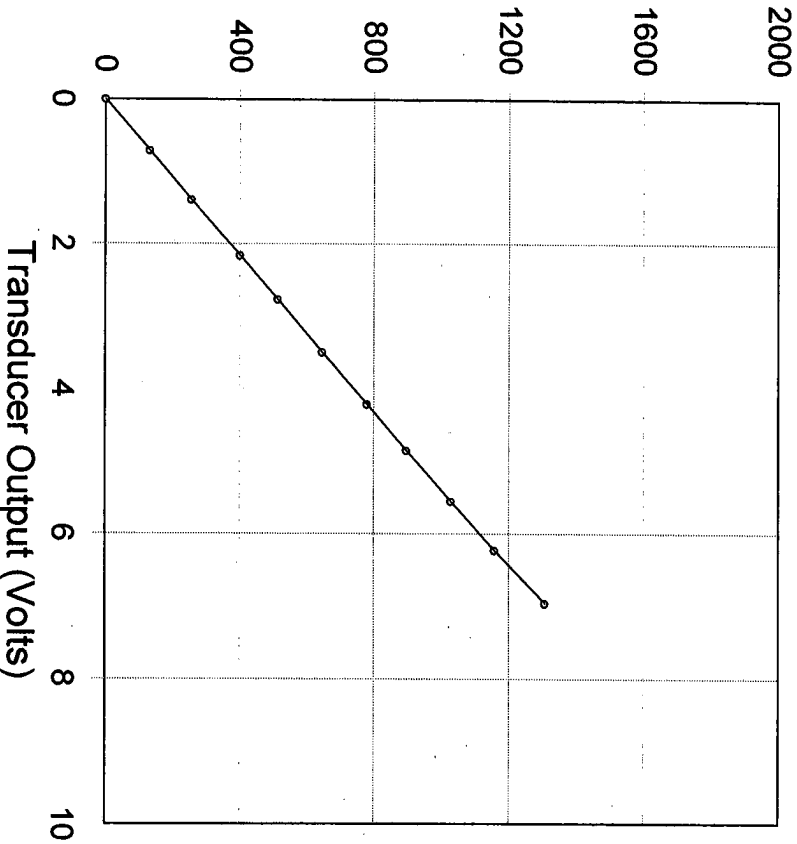

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
131	0.71
254	1.38
400	2.16
512	2.75
643	3.49
777	4.20
895	4.84
1027	5.55
1157	6.23
1307	6.97

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

323.6  $\mu\epsilon/mVV$

Traceable to N.I.S.T.

Calibrated by: Utack

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated on: 21-Aug-2014

Smart Sensor?

Yes

No Smart Chip

Programmed by: UT

Date: 8-21-14

CRC value

8177