


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

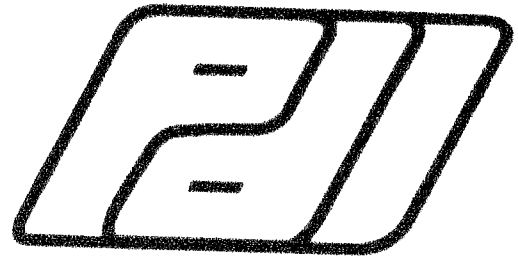

Serial No: K14831 Temperature: 23.1 °C

Model: KICHER PR Humidity: 38%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

419.9 mv/5000g

(84.0 μ v/g)

R²: 0.999955 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 05May2026

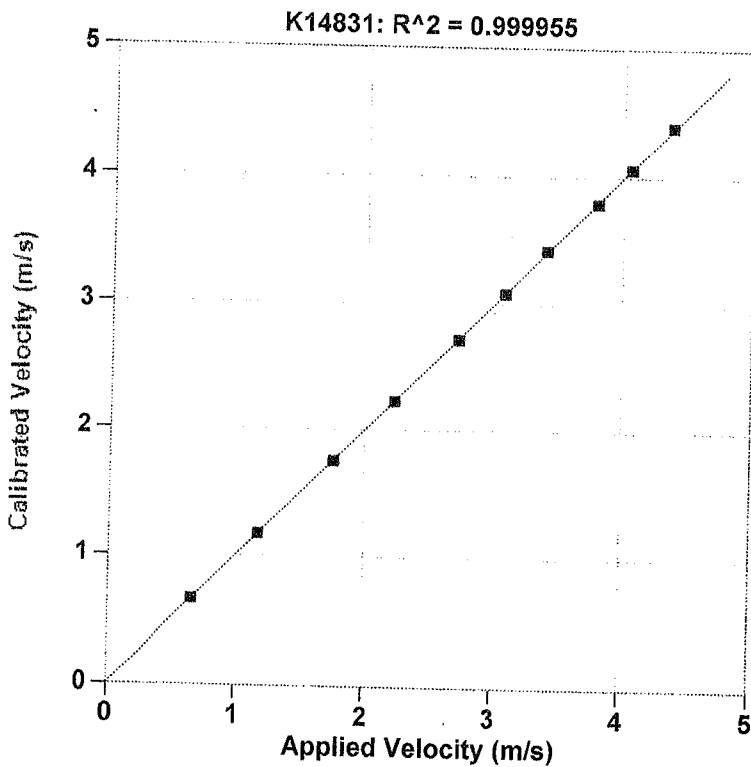

Reference Velocity m/s	S/N K14831 Velocity m/s
0.668	0.666
1.181	1.179
1.765	1.756
2.236	2.232
2.729	2.720
3.088	3.085
3.414	3.423
3.806	3.797
4.067	4.066
4.379	4.395

Maximum Acceleration: 933 g's