

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11091 Temperature: 22.7 °C

Model: PE Humidity: 22%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

929.2 g's/volt

R²: 0.999994 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: JUL 16 2026

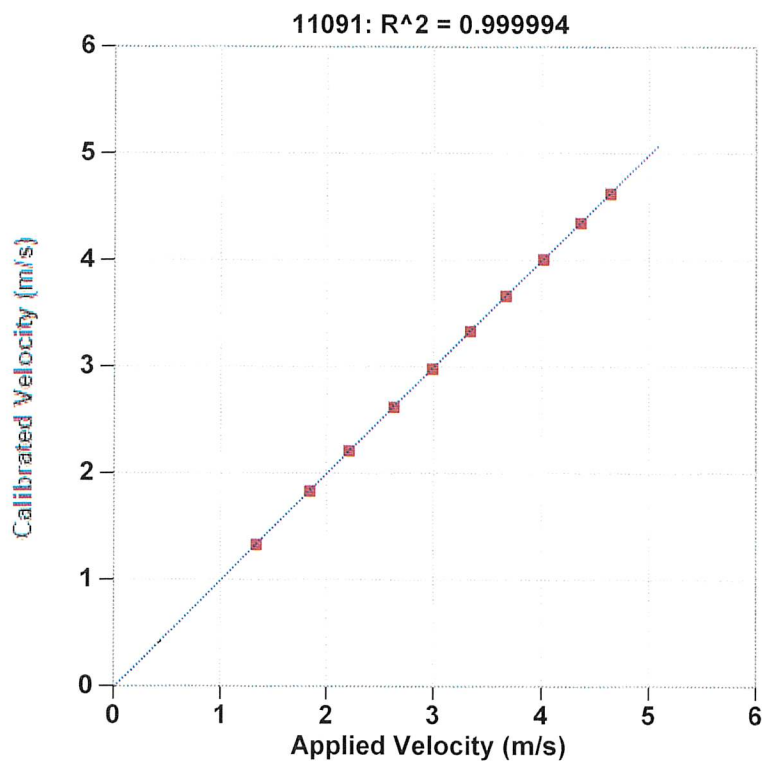

Reference Velocity	S/N 11091 Velocity
m/s	m/s
1.337	1.334
1.838	1.839
2.211	2.215
2.630	2.628
2.986	2.987
3.339	3.342
3.670	3.673
4.014	4.013
4.359	4.356
4.636	4.633
Maximum Acceleration: 1024 g's	