

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11092 Temperature: 22.7 °C

Model: PE Humidity: 22%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

931.4 g's/volt

R^2: 0.999908 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).


Operator: William Johnson


Signed

Calibration valid 2 years

JUL 16 2026

From: _____

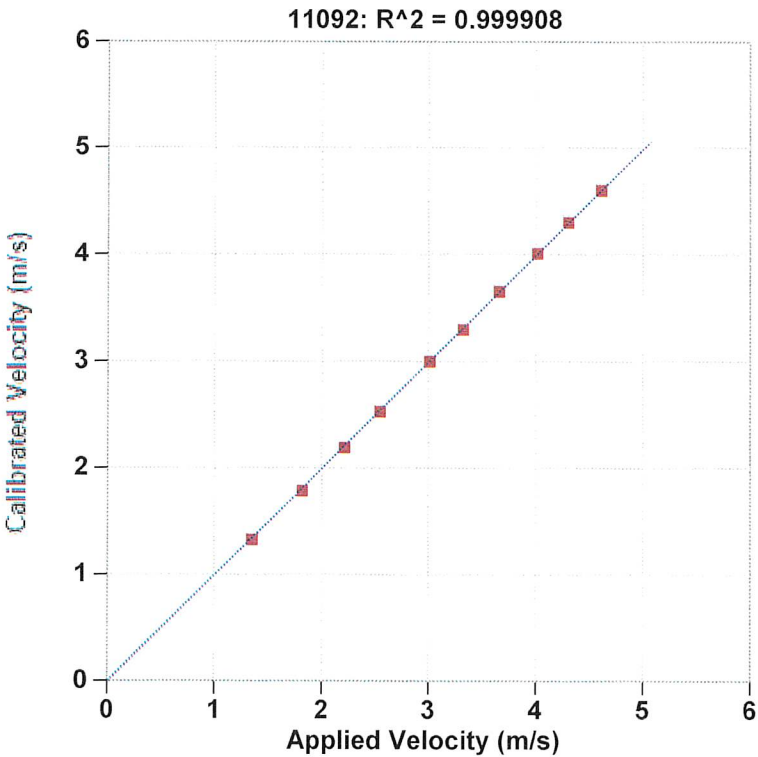

Reference Velocity	S/N 11092 Velocity
m/s	m/s
1.342	1.332
1.808	1.790
2.212	2.197
2.543	2.535
3.006	3.009
3.318	3.310
3.658	3.665
4.014	4.022
4.304	4.314
4.613	4.617
Maximum Acceleration: 1016 g's	