

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11094 Temperature: 22.7 °C

Model: PE Humidity: 22%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR


964.9 g's/volt

R^2: 0.999966 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson




Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

JUL 16 2026

From: _____

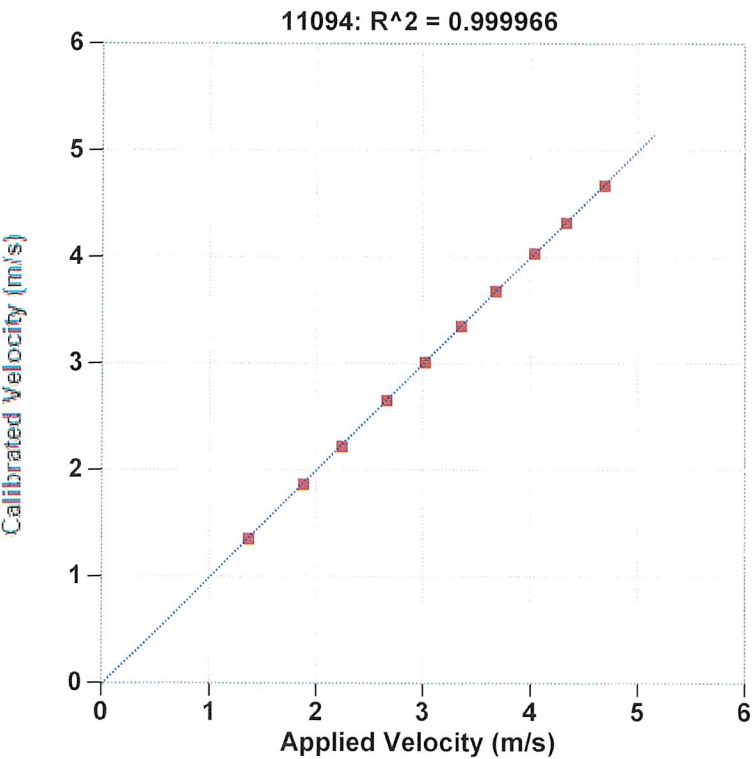

Reference Velocity	S/N 11094 Velocity
m/s	m/s
1.365	1.360
1.881	1.872
2.238	2.227
2.658	2.659
3.016	3.017
3.354	3.355
3.677	3.683
4.030	4.038
4.326	4.327
4.684	4.679
Maximum Acceleration: 1034 g's	