

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11095      Temperature: 21.6 °C  
Model: PE      Humidity: 22%  
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

975.6 g's/volt

R^2: 0.999924 [Chip programmed]


Ref Acc 1: 85363!      Cal on: 14Nov2025  
1000 g's/volt  
Ref Acc 2: 85382!      Cal on: 24Nov2025  
958 g's/volt

Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years  
JUL 16 2026  
From: \_\_\_\_\_

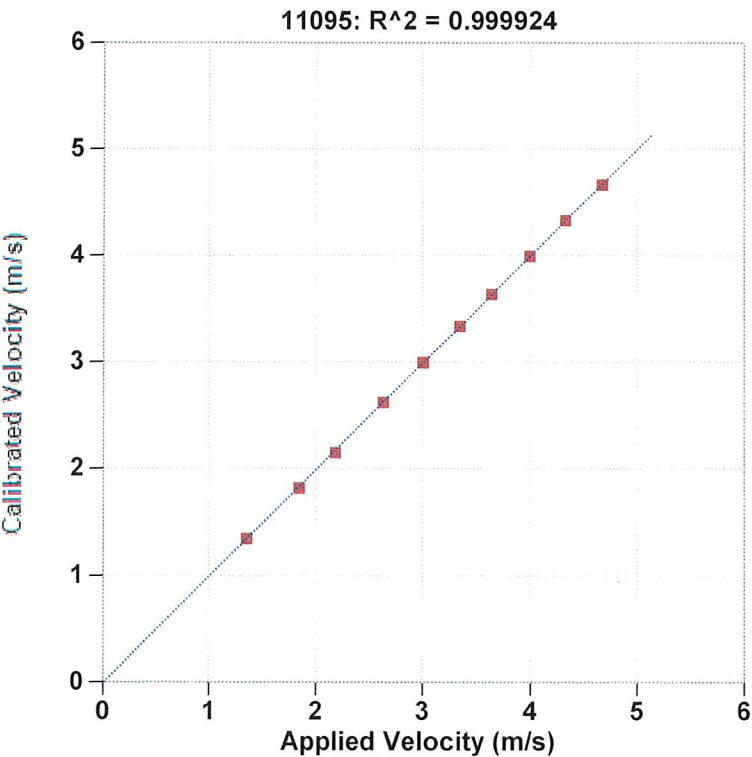

| Reference Velocity | S/N 11095 Velocity |
|--------------------|--------------------|
| m/s                | m/s                |
| 1.347              | 1.353              |
| 1.839              | 1.830              |
| 2.184              | 2.159              |
| 2.630              | 2.629              |
| 3.003              | 3.002              |
| 3.334              | 3.341              |
| 3.637              | 3.640              |
| 3.993              | 3.995              |
| 4.328              | 4.332              |
| 4.668              | 4.668              |

Maximum Acceleration: 1028 g's