

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11096      Temperature: 22.7 °C

Model: PE      Humidity: 22%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

979.9 g's/volt

R^2: 0.999961 [Chip programmed]

Ref Acc 1: 85363!      Cal on: 14Nov2025  
1000 g's/volt

Ref Acc 2: 85382!      Cal on: 24Nov2025  
958 g's/volt

Reference accelerometer calibrations are traceable to  
the United States National Institute of Standards and  
Technology (NIST).

Operator: William Johnson




Signed

Calibration valid 2 years

JUL 16 2026

From: \_\_\_\_\_

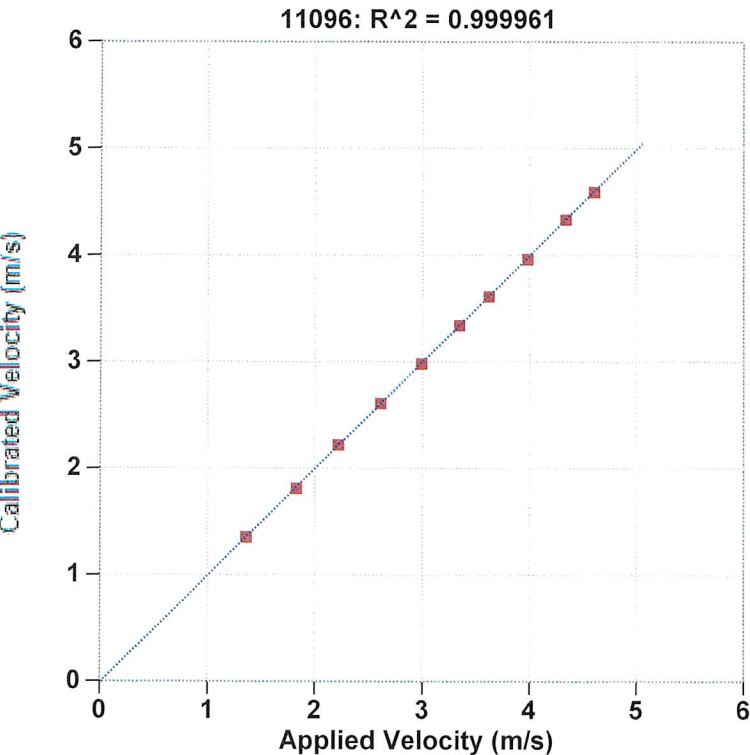

| Reference Velocity | S/N 11096 Velocity |
|--------------------|--------------------|
| m/s                | m/s                |
| 1.355              | 1.356              |
| 1.822              | 1.816              |
| 2.217              | 2.223              |
| 2.600              | 2.613              |
| 2.987              | 2.986              |
| 3.339              | 3.345              |
| 3.615              | 3.616              |
| 3.977              | 3.966              |
| 4.340              | 4.339              |
| 4.603              | 4.601              |

Maximum Acceleration: 1015 g's