


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

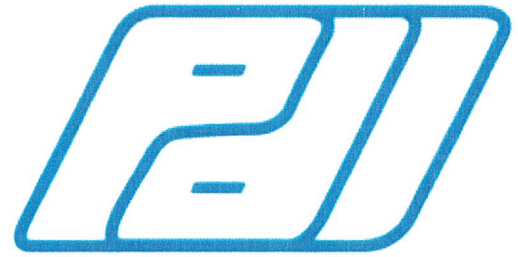

Serial No: 11103 Temperature: 21.9 °C

Model: PE Humidity: 25%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

945.4 g's/volt

R²: 0.999982 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: JUL 16 2026

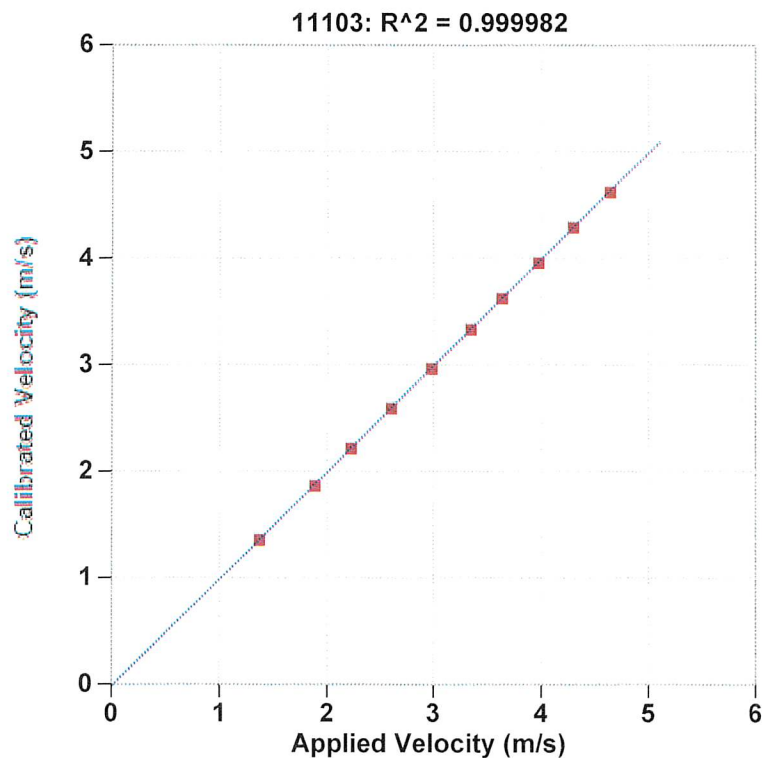

Reference Velocity	S/N 11103 Velocity
m/s	m/s
1.364	1.368
1.882	1.878
2.225	2.229
2.601	2.604
2.979	2.980
3.343	3.345
3.634	3.635
3.973	3.970
4.298	4.304
4.645	4.636
Maximum Acceleration: 1012 g's	