

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11106      Temperature: 22.1 °C

Model: PE      Humidity: 25%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

951.3 g's/volt

R^2: 0.999969 [Chip programmed]

Ref Acc 1: 85363!      Cal on: 14Nov2025  
1000 g's/volt

Ref Acc 2: 85382!      Cal on: 24Nov2025  
958 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to  
the United States National Institute of Standards and  
Technology (NIST).

Calibration valid 2 years

From: JUL 16 2026

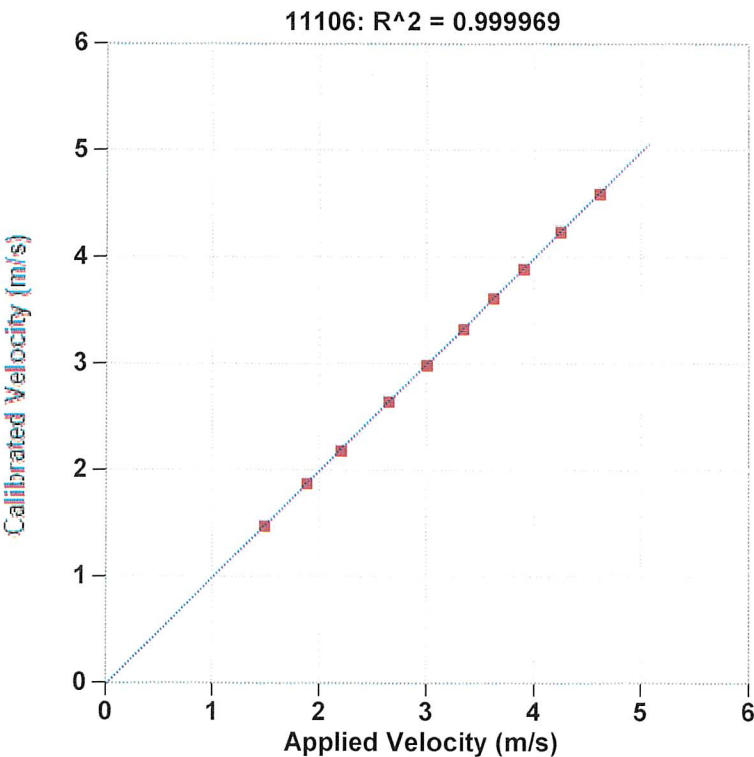

| Reference Velocity             | S/N 11106 Velocity |
|--------------------------------|--------------------|
| m/s                            | m/s                |
| 1.479                          | 1.484              |
| 1.879                          | 1.886              |
| 2.204                          | 2.193              |
| 2.648                          | 2.655              |
| 2.999                          | 2.996              |
| 3.334                          | 3.337              |
| 3.622                          | 3.624              |
| 3.901                          | 3.901              |
| 4.250                          | 4.249              |
| 4.616                          | 4.611              |
| Maximum Acceleration: 1011 g's |                    |