

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 11121 Temperature: 22.4 °C
Model: PE Humidity: 23%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

1032.3 g's/volt

R^2: 0.999955 [Chip programmed]


Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years
JUL 16 2026
From: _____

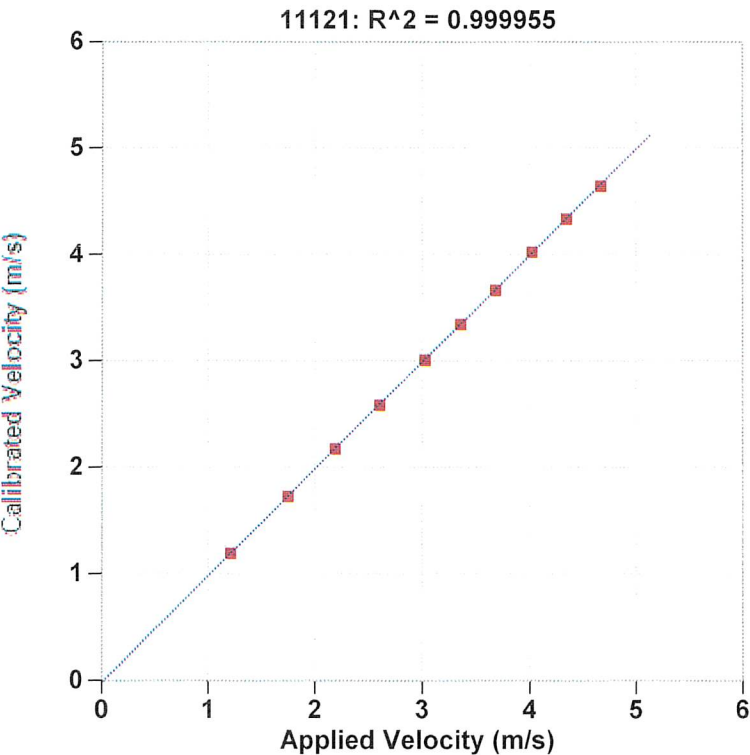

Reference Velocity	S/N 11121 Velocity
m/s	m/s
1.206	1.209
1.744	1.742
2.188	2.187
2.604	2.597
3.022	3.021
3.353	3.357
3.678	3.680
4.020	4.036
4.346	4.346
4.668	4.654

Maximum Acceleration: 1009 g's