


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

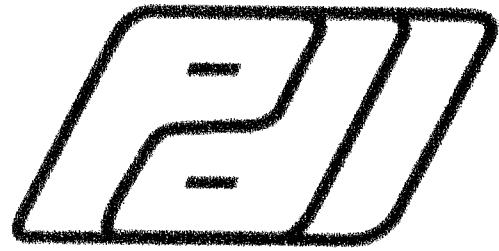

Serial No: 21758 Temperature: 23.3 °C

Model: PIT ACC Humidity: 58%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR


19.1 g's/volt

R²: 0.999960 [No chip]

Ref Acc 1: LW503311! Cal on: 31Jan2024
10 g's/volt

Ref Acc 2: LW503313! Cal on: 31Jan2024
10 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 17Jul2026

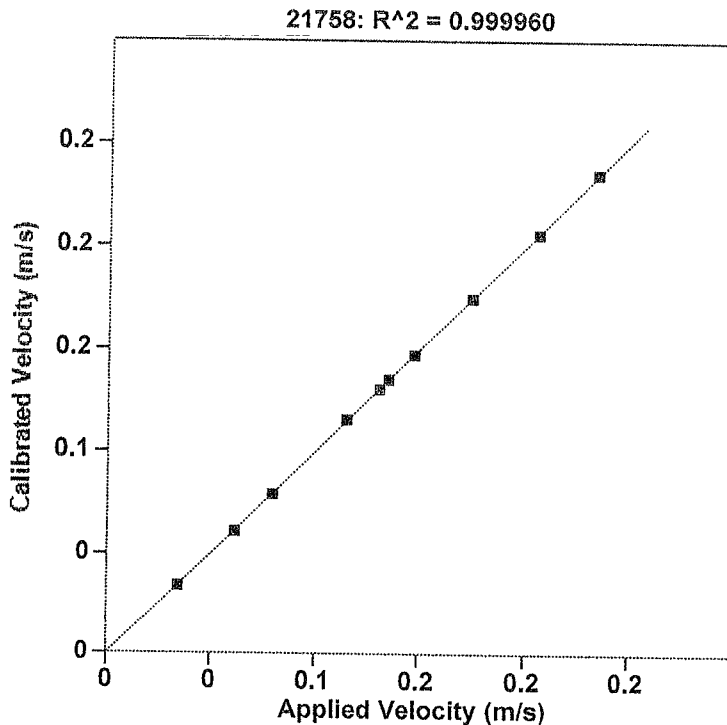

Reference Velocity	S/N 21758 Velocity
m/s	m/s
0.034	0.034
0.061	0.061
0.080	0.079
0.115	0.116
0.131	0.130
0.135	0.135
0.148	0.147
0.175	0.175
0.206	0.206
0.235	0.235
Maximum Acceleration: 28 g's	