


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

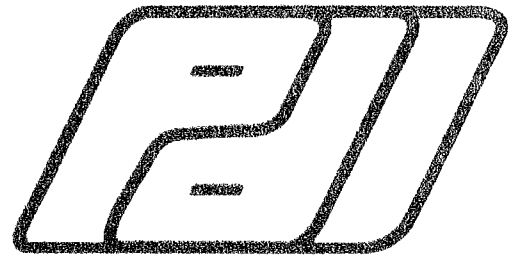

Serial No: 39251 Temperature: 24.6 °C

Model: PE Humidity: 41%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR


1068.0 g's/volt

R²: 0.999992 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 15Jun2026

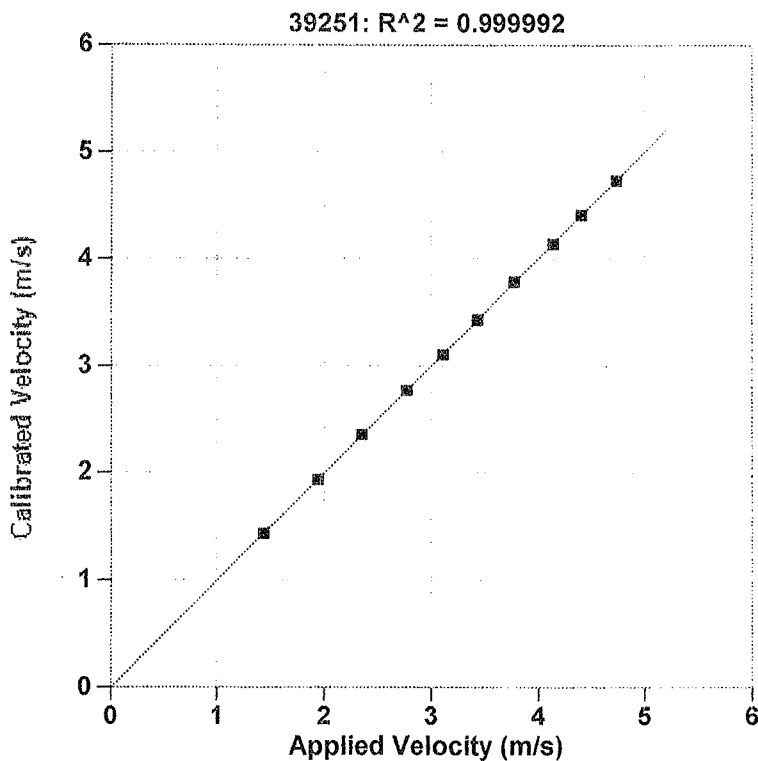

Reference Velocity	S/N 39251 Velocity
m/s	m/s
1.440	1.441
1.946	1.942
2.355	2.359
2.776	2.773
3.114	3.111
3.435	3.436
3.784	3.787
4.143	4.140
4.411	4.414
4.738	4.737
Maximum Acceleration: 1014 g's	