


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

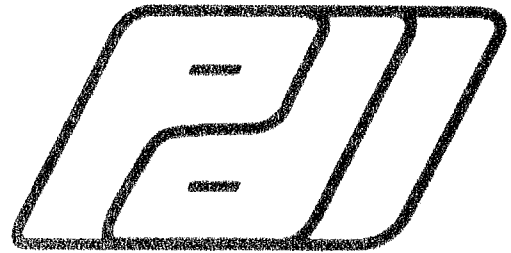

Serial No: 39683 Temperature: 24.9 °C

Model: PE Humidity: 69%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR


1077.8 g's/volt

R²: 0.999985 [No chip]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 09Jun2026

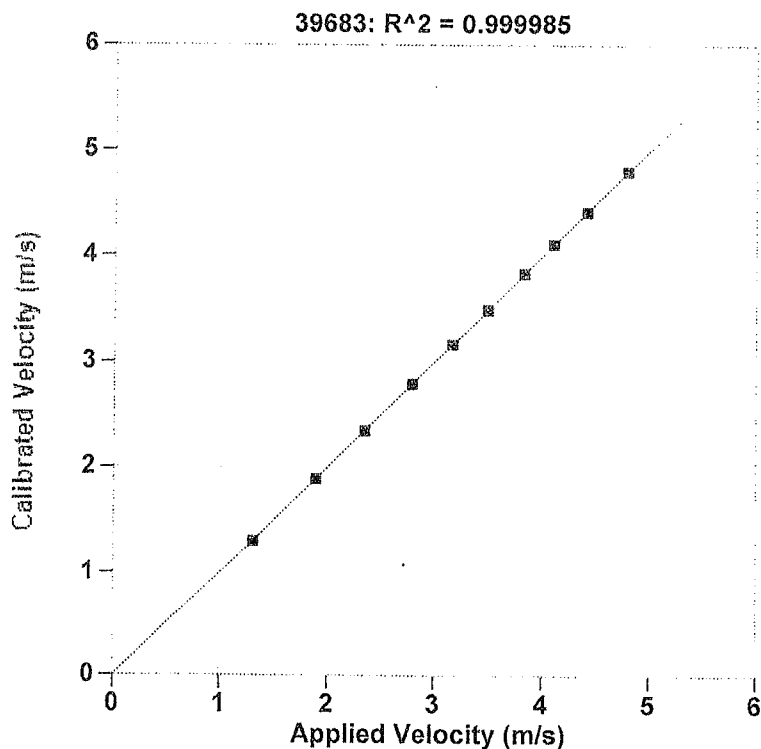

Reference Velocity	S/N 39683 Velocity
m/s	m/s
1.311	1.307
1.897	1.894
2.354	2.345
2.796	2.794
3.174	3.176
3.495	3.498
3.834	3.839
4.112	4.113
4.429	4.425
4.803	4.805
Maximum Acceleration: 1043 g's	