


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

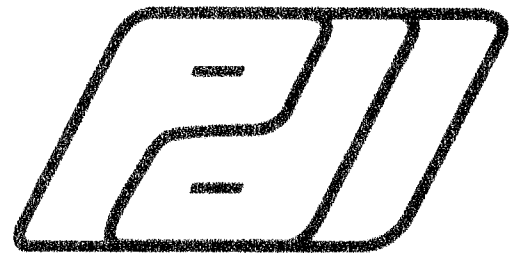

Serial No: 57624 Temperature: 24.5 °C

Model: PE Humidity: 41%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

960.0 g's/volt

R²: 0.999994 [Chip programmed]

Ref Acc 1: 853631 Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 853821 Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 07Jul2026

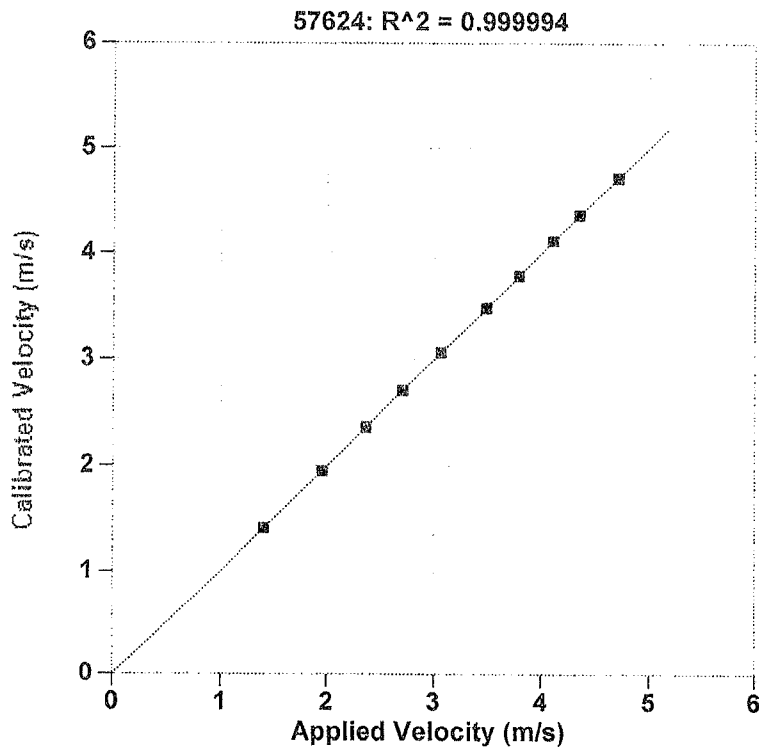

Reference Velocity	S/N 57624 Velocity
m/s	m/s
1.415	1.412
1.962	1.958
2.371	2.370
2.716	2.714
3.071	3.070
3.489	3.490
3.795	3.797
4.119	4.121
4.369	4.372
4.722	4.720

Maximum Acceleration: 1032 g's