


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

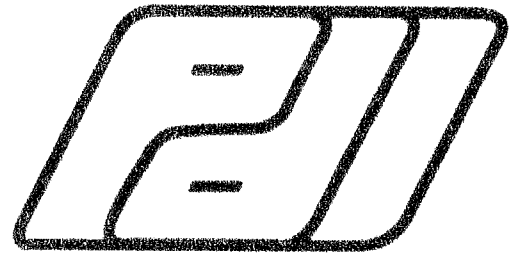

Serial No: 58389 Temperature: 24.5 °C

Model: PE Humidity: 41%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR


1045.4 g's/volt

R^2: 0.999993 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 07Jul2026

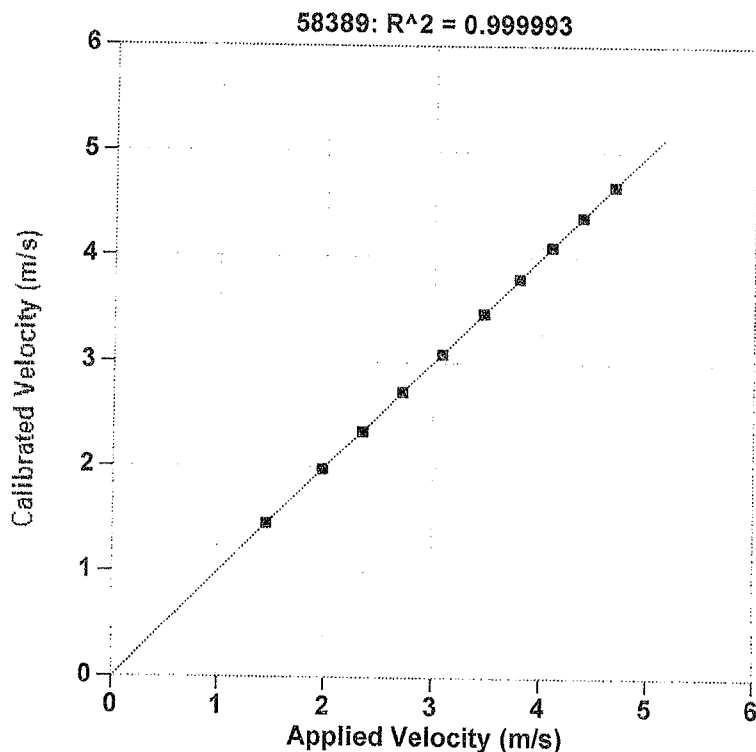

Reference Velocity	S/N 58389 Velocity
m/s	m/s
1.461	1.461
1.987	1.983
2.342	2.339
2.720	2.719
3.083	3.082
3.468	3.471
3.795	3.800
4.098	4.098
4.384	4.385
4.683	4.681
Maximum Acceleration: 1026 g's	