


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

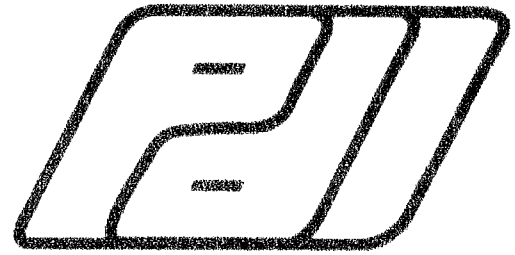

Serial No: 73855 Temperature: 26.3 °C

Model: PE Humidity: 51%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1027.4 g's/volt

R²: 0.999982 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 01Jul2026

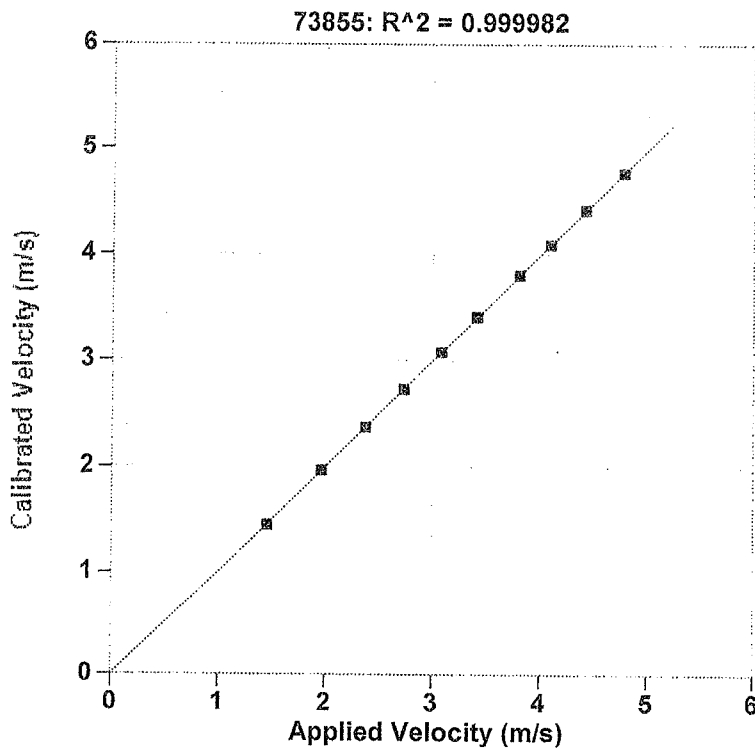

Reference Velocity	S/N 73855 Velocity
m/s	m/s
1.456	1.452
1.970	1.971
2.380	2.378
2.738	2.735
3.084	3.083
3.406	3.413
3.808	3.811
4.103	4.101
4.430	4.436
4.788	4.781
Maximum Acceleration: 1062 g's	