


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

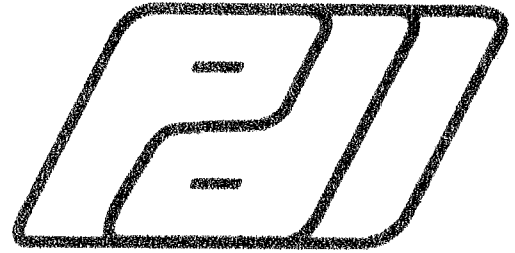

Serial No: 73857 Temperature: 26.3 °C

Model: PE Humidity: 51%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR


1061.6 g's/volt

R²: 0.999994 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 01Jul2026

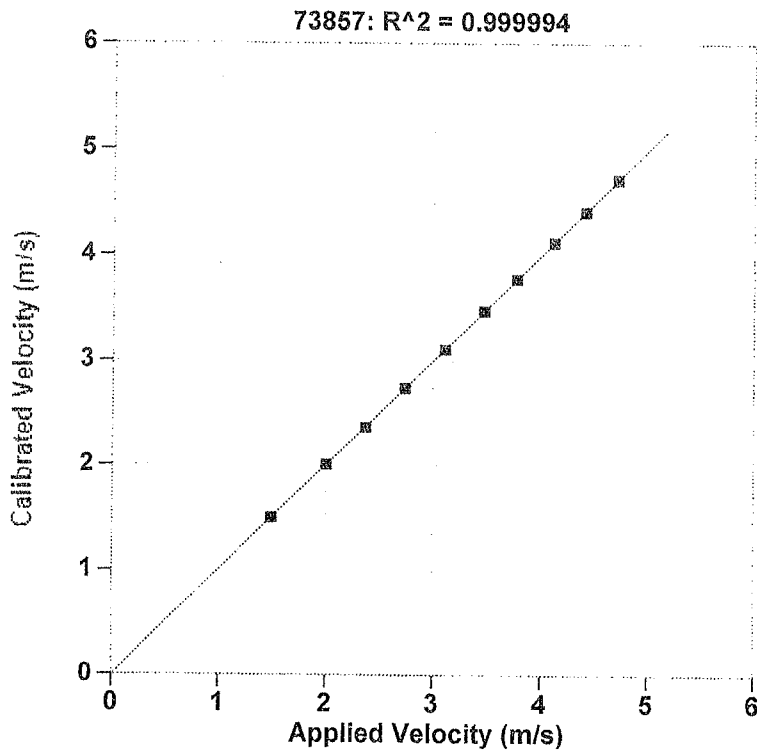

Reference Velocity	S/N 73857 Velocity
m/s	m/s
1.500	1.497
2.011	2.012
2.375	2.369
2.745	2.744
3.114	3.113
3.478	3.480
3.783	3.783
4.127	4.127
4.426	4.425
4.724	4.728
Maximum Acceleration: 1052 g's	