


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

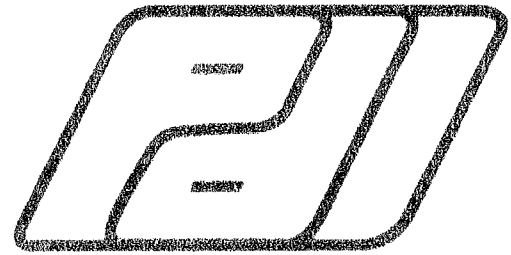

Serial No: K12070 Temperature: 24.5 °C

Model: KICHER PR Humidity: 42%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

434.6 mv/5000g


(86.9 μ v/g)

R²: 0.999964 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Calibration valid 2 years

From: 07Jul2026

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

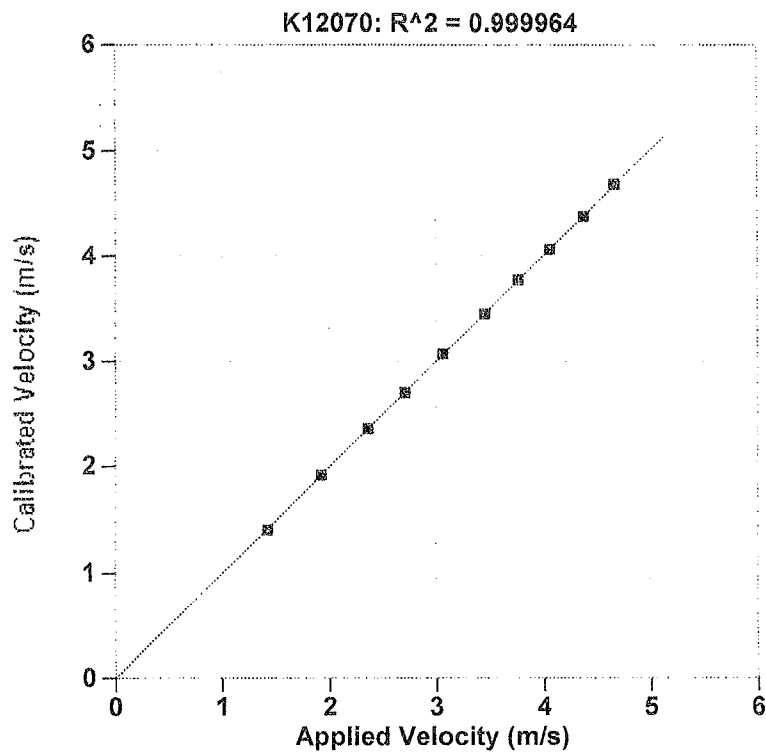

Reference Velocity	S/N K12070 Velocity
m/s	m/s
1.422	1.410
1.930	1.925
2.366	2.362
2.714	2.708
3.069	3.073
3.459	3.456
3.772	3.775
4.064	4.063
4.387	4.386
4.676	4.687

Maximum Acceleration: 1026 g's