


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

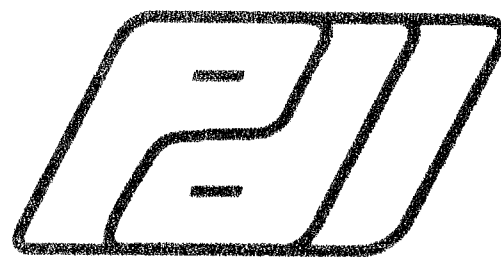

Serial No: K12274 Temperature: 25.7 °C

Model: KICHER PR Humidity: 50%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

403.8 mv/5000g

(80.8 μ v/g)

R²: 0.999939 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 01Jul2026

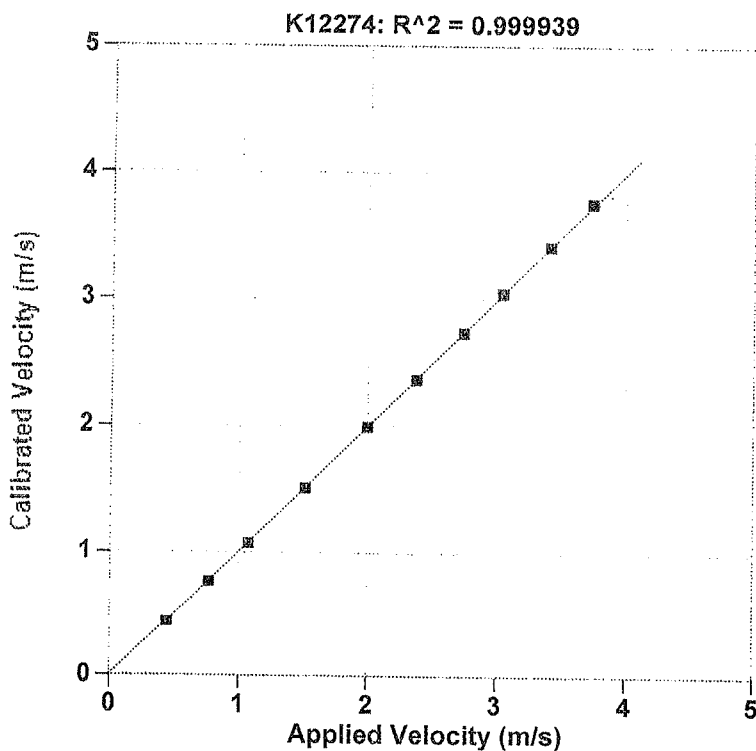

Reference Velocity	S/N K12274 Velocity
m/s	m/s
0.443	0.437
0.772	0.764
1.082	1.075
1.519	1.516
2.003	1.998
2.381	2.374
2.750	2.741
3.052	3.052
3.418	3.418
3.746	3.766

Maximum Acceleration: 819 g's