

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15378 Temperature: 26.5 °C

Model: KICHER PR Humidity: 51%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

416.8 mv/5000g


(83.4 μ v/g)

R²: 0.999932 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: **JUL 17 2026**

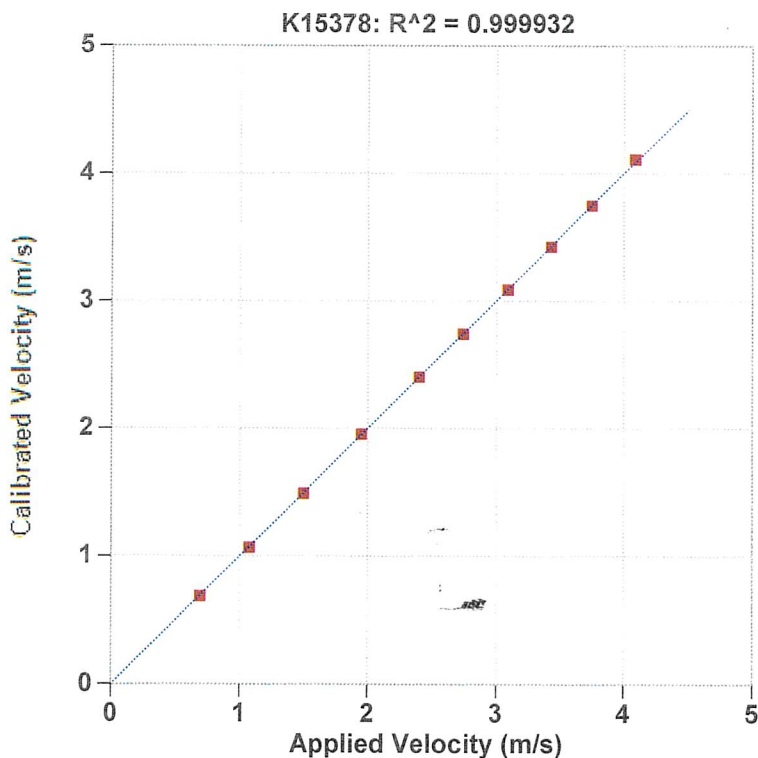

Reference Velocity	S/N K15378 Velocity
m/s	m/s
0.703	0.694
1.083	1.073
1.501	1.495
1.956	1.959
2.406	2.408
2.749	2.744
3.095	3.092
3.435	3.427
3.758	3.753
4.092	4.114
Maximum Acceleration: 905 g's	