


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

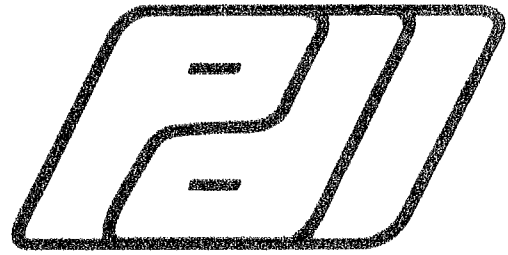

Serial No: K3222 Temperature: 24.2 °C

Model: KICHER PR Humidity: 42%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

345.6 mv/5000g

(69.1 μ v/g)

R²: 0.999973 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 15Jun2026

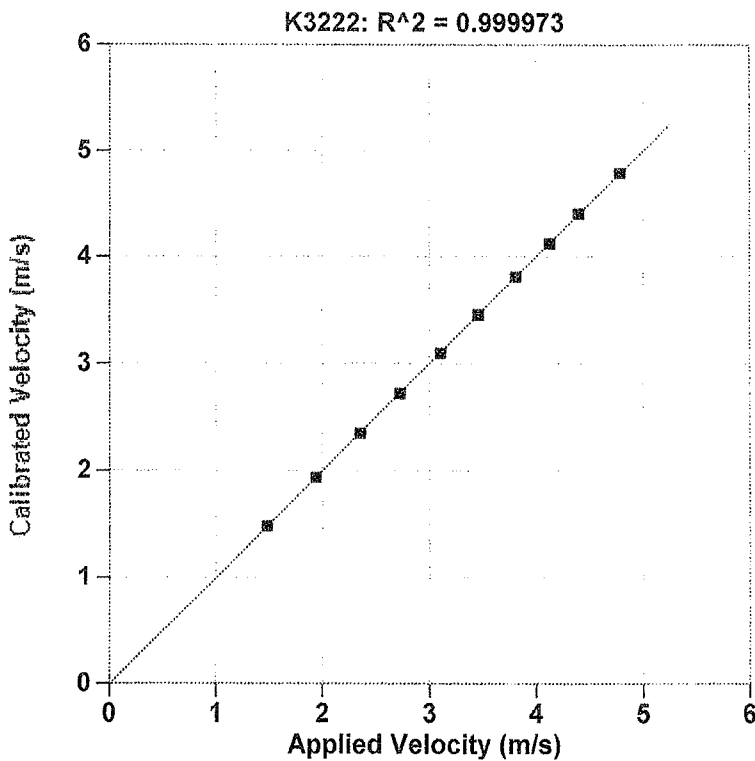

Reference Velocity	S/N K3222 Velocity
m/s	m/s
1.482	1.482
1.942	1.939
2.363	2.353
2.733	2.725
3.105	3.102
3.462	3.462
3.815	3.815
4.133	4.131
4.408	4.414
4.791	4.798

Maximum Acceleration: 1026 g's