

Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.




Serial No: K3799 Temperature: 23.8 °C
Model: PR Humidity: 56%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

308.9 mv/5000g
(61.8 μ v/g)
R²: 0.999967 [Chip programmed]

Ref Acc 1: 78268! Cal on: 11Jan2024
986 g's/volt
Ref Acc 2: 78270! Cal on: 11Jan2024
971 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 17Jul2026

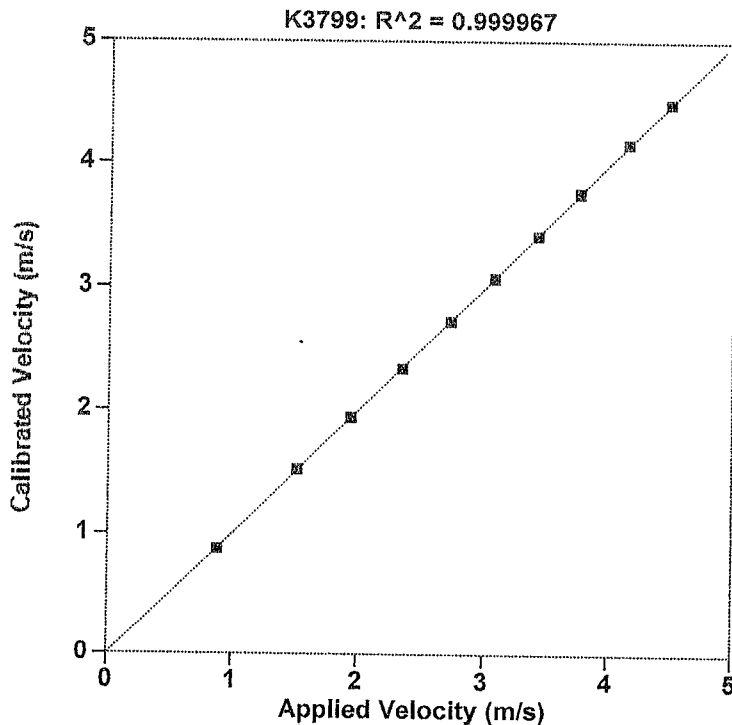

Reference Velocity	S/N K3799 Velocity
m/s	m/s
0.880	0.872
1.516	1.519
1.943	1.939
2.352	2.342
2.730	2.725
3.076	3.073
3.426	3.420
3.763	3.766
4.149	4.159
4.483	4.489
Maximum Acceleration: 959 g's	