


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

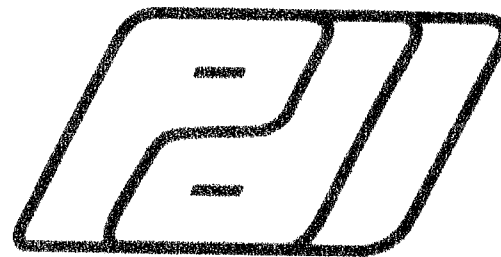

Serial No: LW383807 Temperature: 24.2 °C

Model: PIT ACC Humidity: 40%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

9.9 g's/volt

R²: 0.999989 [Chip programmed]

Ref Acc 1: LW547723! Cal on: 21Oct2025
10 g's/volt

Ref Acc 2: LW547722! Cal on: 21Oct2025
10 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 08Jul2026

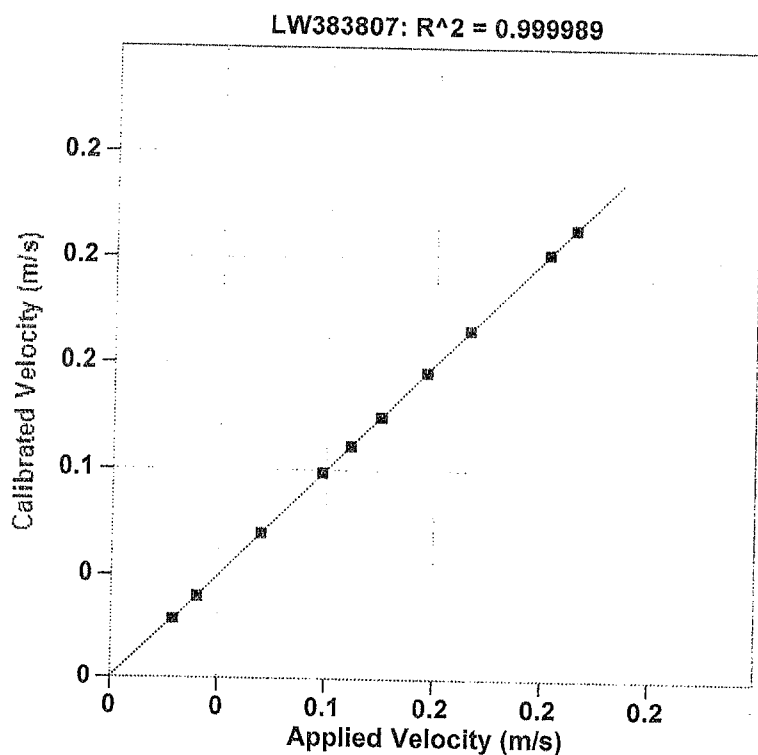

Reference Velocity	S/N LW383807 Velocity
m/s	m/s
0.029	0.029
0.040	0.040
0.070	0.070
0.098	0.099
0.112	0.111
0.125	0.125
0.146	0.146
0.166	0.166
0.203	0.203
0.215	0.215

Maximum Acceleration: 25 g's