


# Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

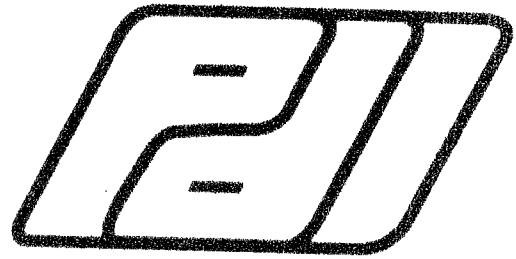

Serial No: LW408923      Temperature: 24.5 °C

Model: PIT ACC      Humidity: 35%

Calibrated on: Channel 3 on 8G 5161 LE

## PDA CALIBRATION FACTOR


10.1 g's/volt

R<sup>2</sup>: 0.999953 [Chip programmed]

Ref Acc 1: LW547723!      Cal on: 21Oct2025  
10 g's/volt

Ref Acc 2: LW547722!      Cal on: 21Oct2025  
10 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to  
the United States National Institute of Standards and  
Technology (NIST).

Calibration valid 2 years

From: 16Jul2026

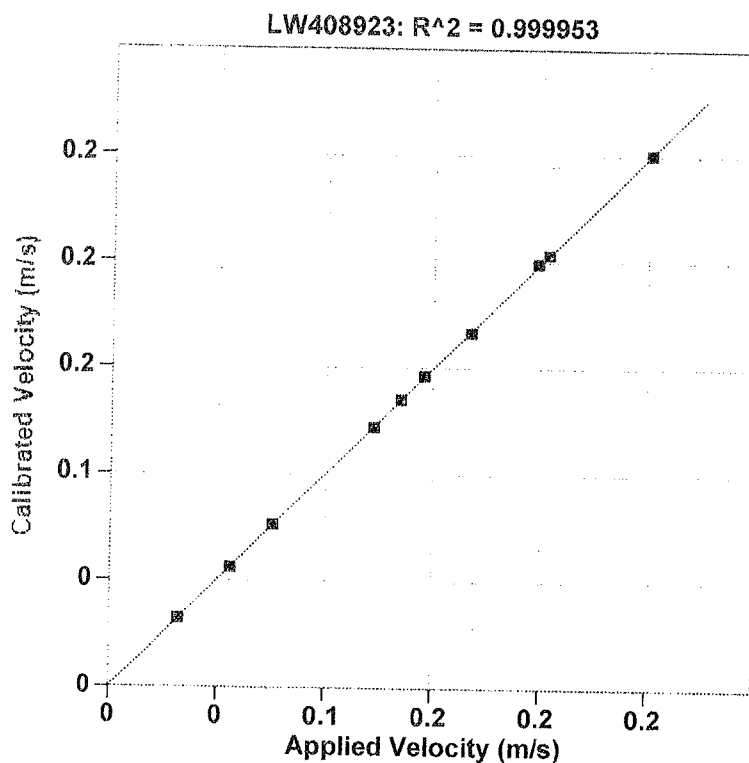

| Reference Velocity | S/N LW408923 Velocity |
|--------------------|-----------------------|
| m/s                | m/s                   |
| 0.032              | 0.032                 |
| 0.056              | 0.056                 |
| 0.076              | 0.076                 |
| 0.122              | 0.122                 |
| 0.135              | 0.135                 |
| 0.146              | 0.146                 |
| 0.168              | 0.167                 |
| 0.199              | 0.200                 |
| 0.204              | 0.204                 |
| 0.251              | 0.251                 |

Maximum Acceleration: 30 g's