

Pile Dynamics, Inc.


Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: P333
PDI Gage Factor: 95.1
Mean Linear Correlation Coefficient: 0.999969

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2303.1	-6.864	597.1	2.202
-1804.5	-5.297	1023.6	3.526
-1279.5	-3.718	1417.3	4.770
-748.0	-2.064	1804.5	5.945
-288.7	-0.587	2001.3	6.539
157.5	0.825		

Calibration Curve

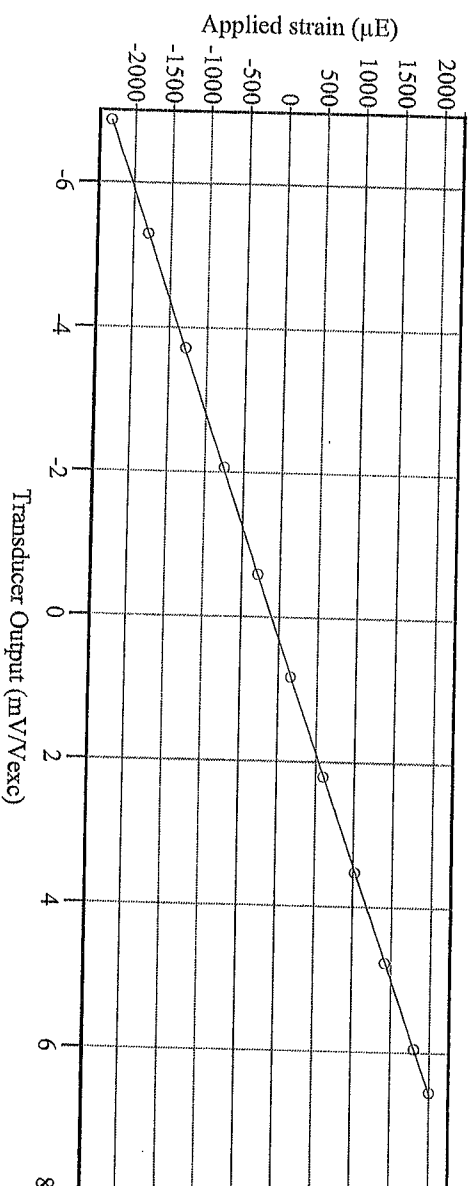

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman
PDI Gage: P333
Calibration Date: 6/25/2026 6:18:34 AM
Calibration valid 2 years

Signature:

Paul Hartman



Pile Dynamics, Inc.