




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: T349
 PDI Gage Factor: 147.0
 Mean Linear Correlation Coefficient: 0.999925

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2047.2	-4.170	570.9	1.106
-1548.6	-3.163	984.3	1.927
-1049.9	-2.202	1371.4	2.721
-577.4	-1.274	1758.5	3.500
-183.7	-0.467	2001.3	3.986
190.3	0.321		

Calibration Curve

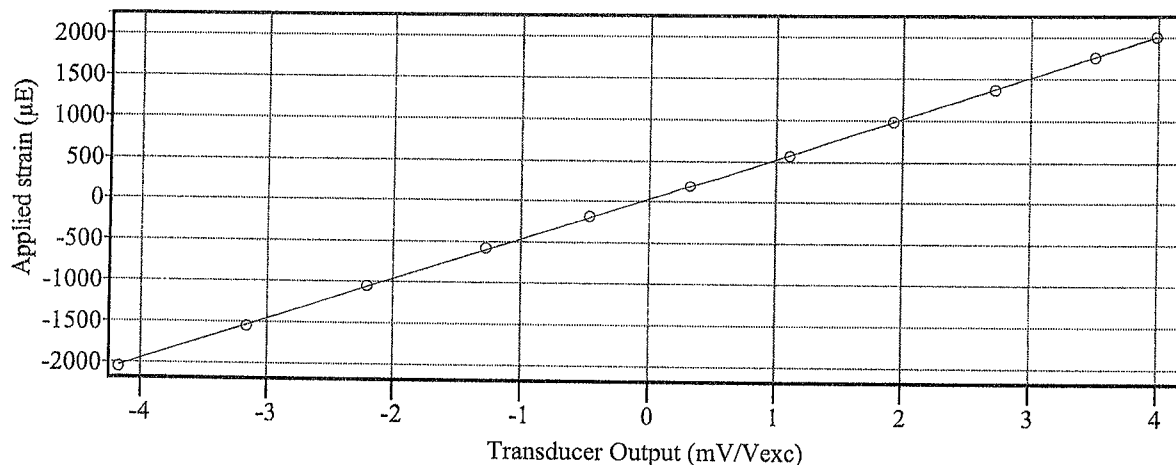

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

PDI Gage: T349

Calibration Date: 7/14/2026 9:08:27 AM

Calibration valid 2 years

Signature:

Paul Hartman

