




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: U863
 PDI Gage Factor: 145.6
 Mean Linear Correlation Coefficient: 0.999939

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2368.8	-4.918	524.9	1.040
-1817.6	-3.767	925.2	1.848
-1318.9	-2.703	1305.8	2.610
-839.9	-1.736	1653.5	3.325
-334.6	-0.708	2021.0	4.048
109.4	0.192		

Calibration Curve

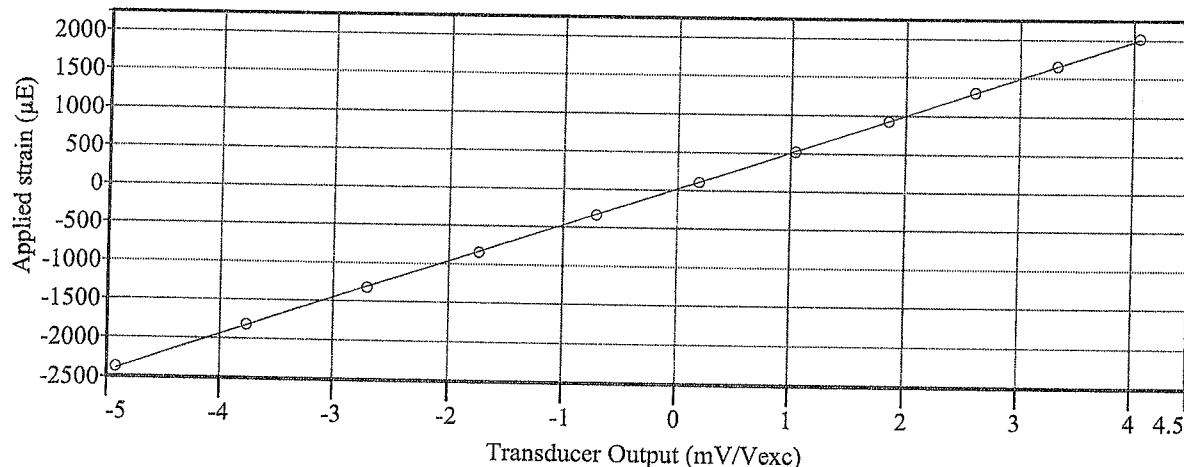

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: U863

Calibration Date: 6/25/2026 6:54:46 AM

Calibration valid 2 years

