




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: V787
PDI Gage Factor: 92.1
Mean Linear Correlation Coefficient: 0.999809

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1922.6	-6.391	387.1	1.148
-1496.1	-5.003	724.0	2.301
-1115.5	-3.713	1076.1	3.388
-721.8	-2.417	1406.4	4.414
-380.6	-1.285	1732.3	5.414
6.6	-0.067	1988.2	6.191

Calibration Curve

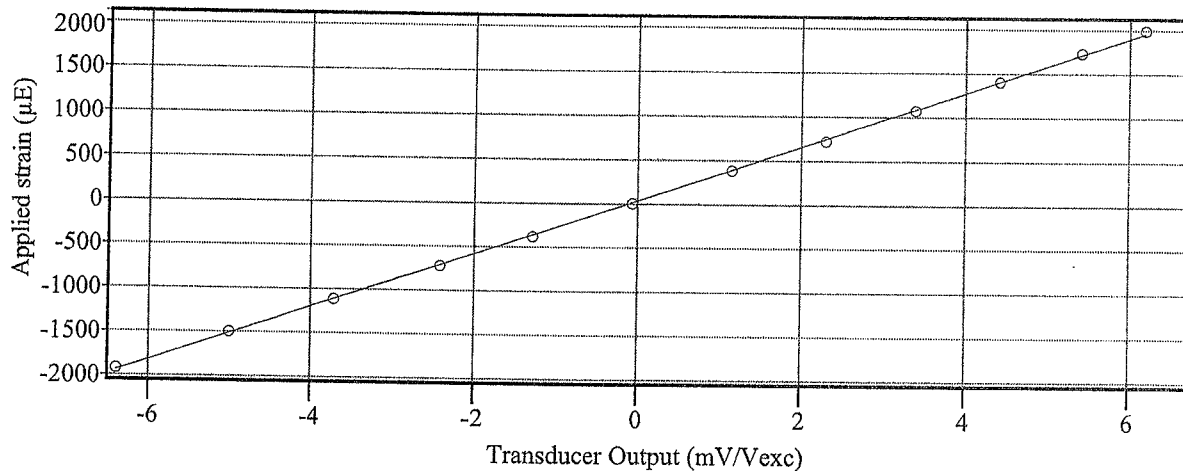

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

PDI Gage: V787

Calibration Date: 6/23/2026 9:10:08 AM

Calibration valid 2 years

Signature: _____

Paul Hartman

