




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: V846
 PDI Gage Factor: 92.2
 Mean Linear Correlation Coefficient: 0.999534

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2255.0	-7.334	282.2	1.044
-1732.3	-5.661	597.1	2.022
-1209.5	-4.001	958.0	3.041
-708.7	-2.393	1312.3	4.127
-315.0	-1.067	1666.7	5.220
-6.6	0.039	1981.6	6.246

Calibration Curve

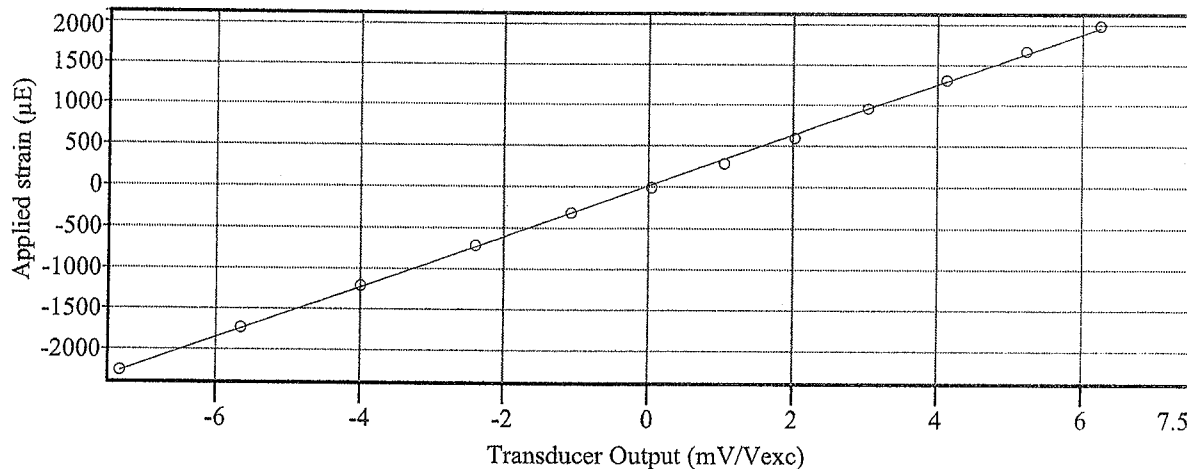


PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: 

PDI Gage: V846

Calibration Date: 6/23/2026 9:18:32 AM

Calibration valid 2 years

