




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: V848
PDI Gage Factor: 95.2
Mean Linear Correlation Coefficient: 0.999831

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2257.2	-7.095	419.9	1.247
-1830.7	-5.764	800.5	2.494
-1364.8	-4.421	1181.1	3.647
-866.1	-2.875	1542.0	4.738
-374.0	-1.336	1896.3	5.783
19.7	-0.027	1994.8	6.063

Calibration Curve

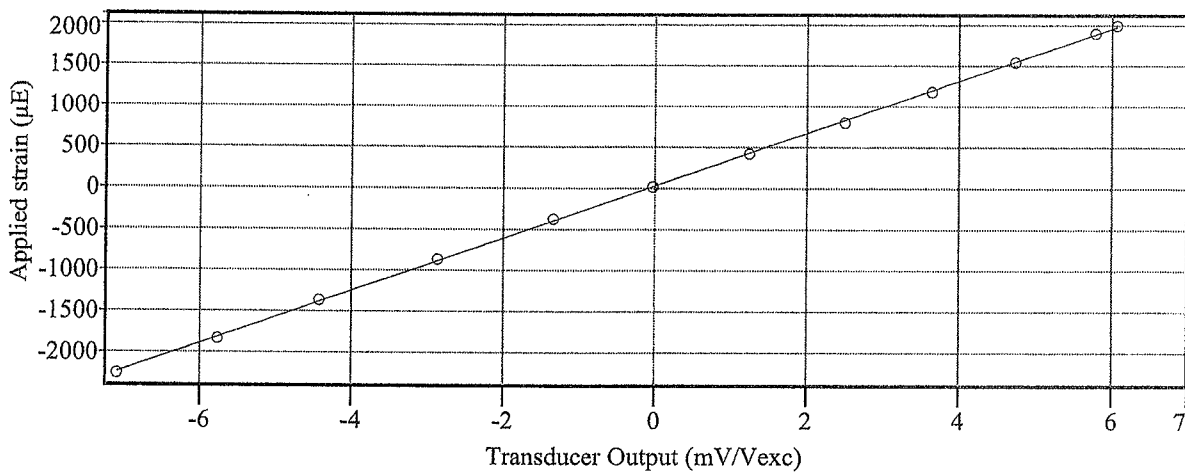

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

PDI Gage: V848

Calibration Date: 6/23/2026 9:26:10 AM

Calibration valid 2 years

Signature: _____

Paul Hartman

