




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: Z672
PDI Gage Factor: 95.7
Mean Linear Correlation Coefficient: 0.999715

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2329.4	-7.291	511.8	1.715
-1778.2	-5.511	918.6	2.946
-1338.6	-4.031	1292.7	4.072
-833.3	-2.443	1647.0	5.131
-341.2	-0.940	2007.9	6.185
85.3	0.407		

Calibration Curve

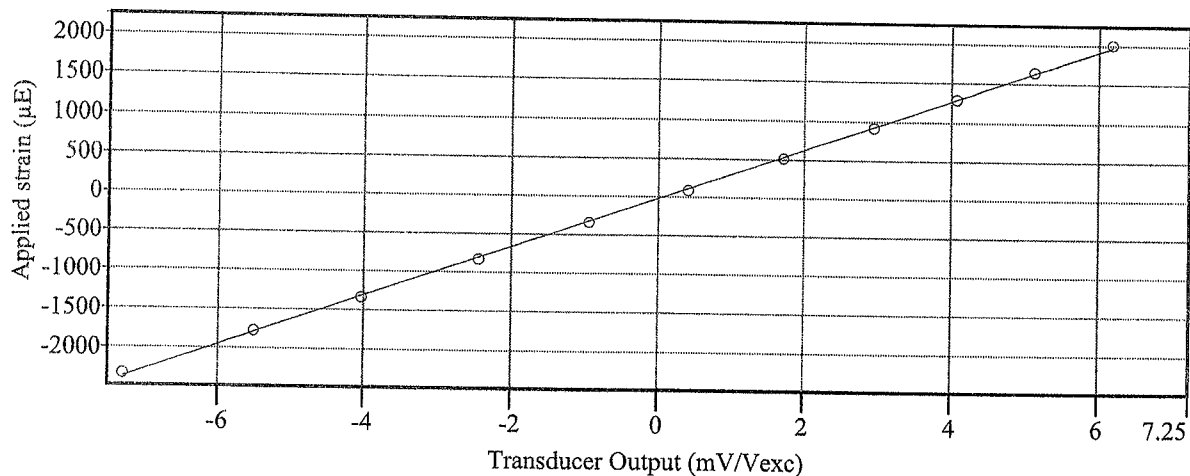

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

PDI Gage: Z672

Calibration Date: 6/26/2026 12:57:28 PM

Calibration valid 2 years

Signature:

Paul Hartman

