


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

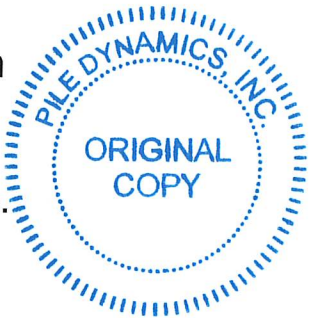

Serial No: 00013 Temperature: 20.8 °C
Model: PR Humidity: 49%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

587.7 mv/5000g
(117.5 μv/g)
R^2: 0.999987 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: AUG 28 2026

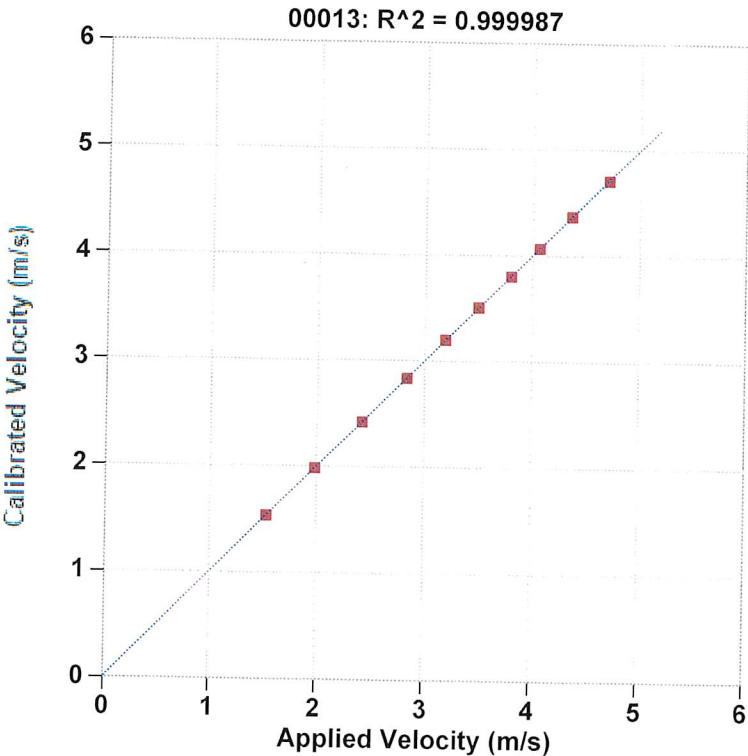

Reference Velocity	S/N 00013 Velocity
m/s	m/s
1.532	1.531
1.981	1.979
2.416	2.416
2.833	2.834
3.191	3.196
3.496	3.501
3.800	3.797
4.061	4.062
4.362	4.364
4.712	4.705

Maximum Acceleration: 1037 g's