


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

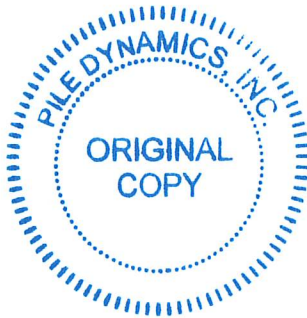

Serial No: 00014 Temperature: 20.8 °C
Model: PR Humidity: 49%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

865.2 mv/5000g
(173.0 μv/g)
R^2: 0.999989 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 9202 8 2 NOV

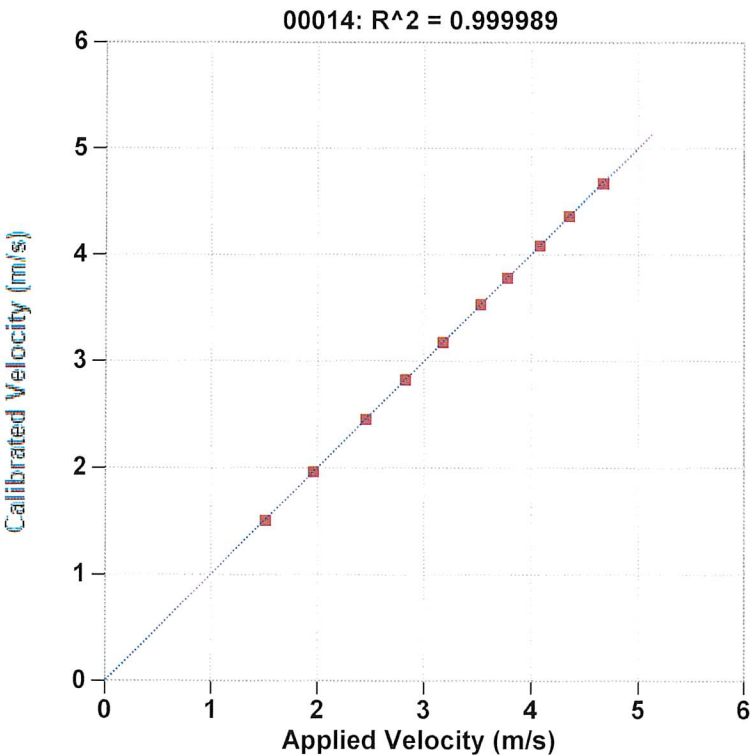

Reference Velocity	S/N 00014 Velocity
m/s	m/s
1.511	1.504
1.959	1.961
2.457	2.453
2.822	2.823
3.174	3.174
3.527	3.530
3.778	3.778
4.080	4.083
4.355	4.358
4.675	4.671

Maximum Acceleration: 1028 g's