

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 00015 Temperature: 20.8 °C

Model: PR Humidity: 49%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

953.0 mv/5000g
(190.6 µv/g)
R^2: 0.999988 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

[Signature]
Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: **AUG 28 2026**

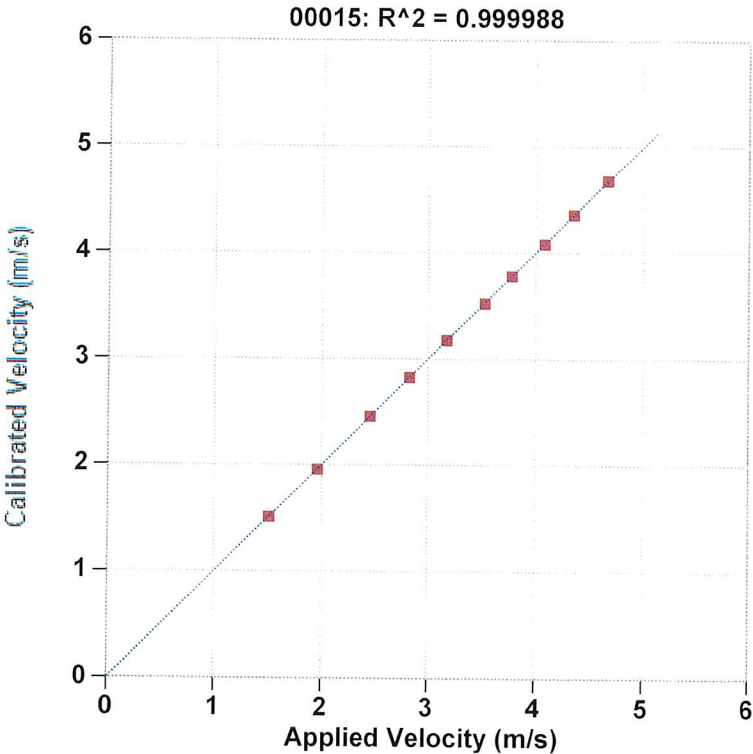

Reference Velocity	S/N 00015 Velocity
m/s	m/s
1.511	1.508
1.959	1.955
2.457	2.456
2.822	2.823
3.174	3.175
3.527	3.519
3.778	3.778
4.080	4.080
4.355	4.357
4.675	4.680
Maximum Acceleration: 1028 g's	