


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

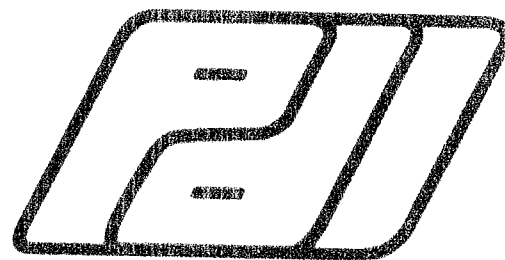

Serial No: 13775 Temperature: 24.2 °C

Model: PE Humidity: 42%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

990.2 g's/volt

R²: 0.999961 [No chip]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson


William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 10Aug2026

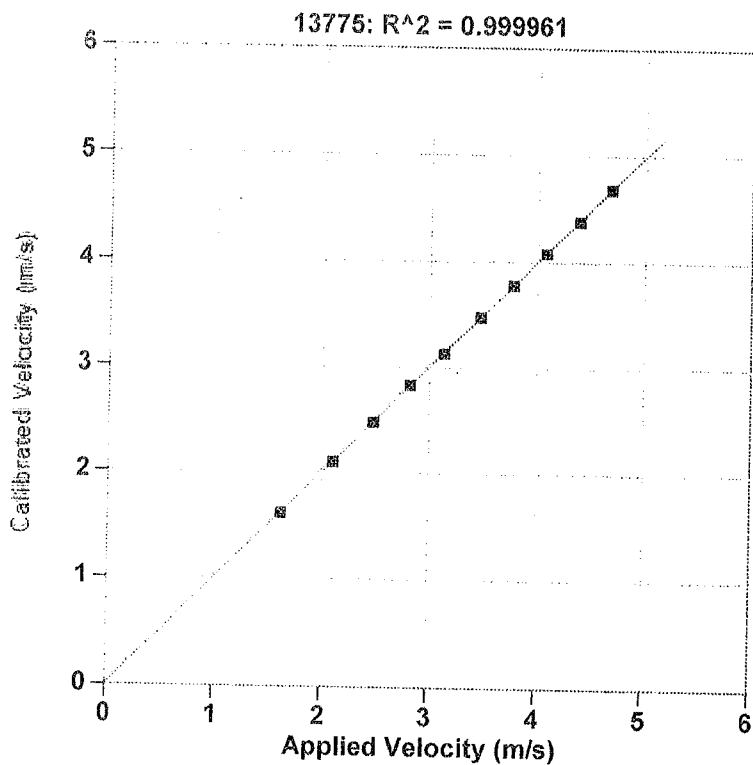

Reference Velocity	S/N 13775 Velocity
m/s	m/s
1.617	1.611
2.102	2.093
2.479	2.474
2.821	2.823
3.132	3.128
3.465	3.476
3.767	3.774
4.082	4.080
4.391	4.387
4.687	4.689
Maximum Acceleration: 1031 g's	