




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 2756W
 PDI Gage Factor: 104.1
 Mean Linear Correlation Coefficient: 0.999611

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1955.4	-5.162	271.2	1.180
-1509.2	-3.851	551.2	1.944
-1049.9	-2.548	826.8	2.706
-715.2	-1.591	1122.0	3.480
-446.2	-0.805	1406.4	4.244
-65.6	0.257	1961.9	5.679

Calibration Curve

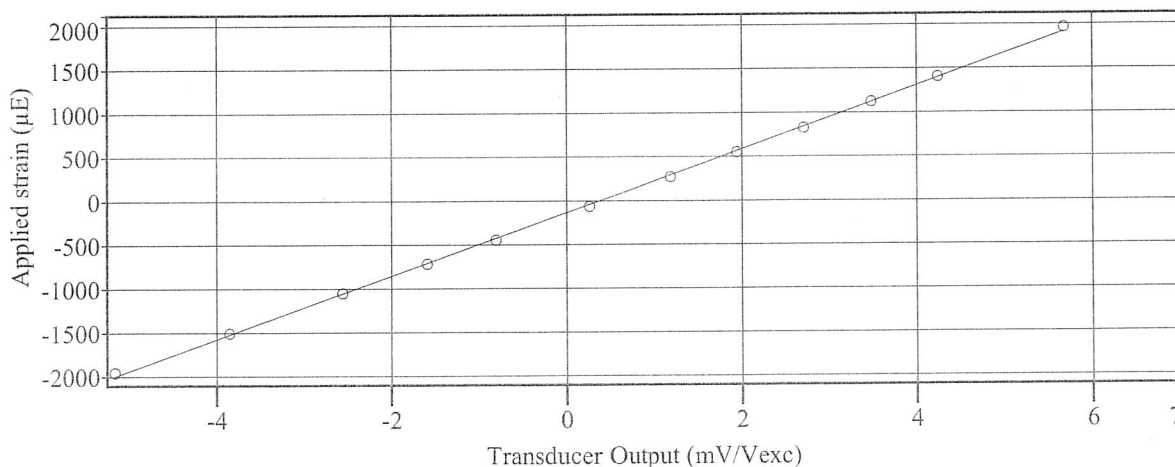

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal
 PDI Gage: 2756W
 Calibration Date:
 Calibration valid 2 years

Signature:

AUG 27 2026

