




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 2759W
PDI Gage Factor: 97.3
Mean Linear Correlation Coefficient: 0.999970

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2187.2	-6.421	708.7	2.163
-1640.4	-4.808	1036.7	3.146
-1069.6	-3.132	1351.7	4.102
-505.2	-1.468	1697.3	5.099
-91.9	-0.248	1988.2	5.925
282.2	0.872		

Calibration Curve

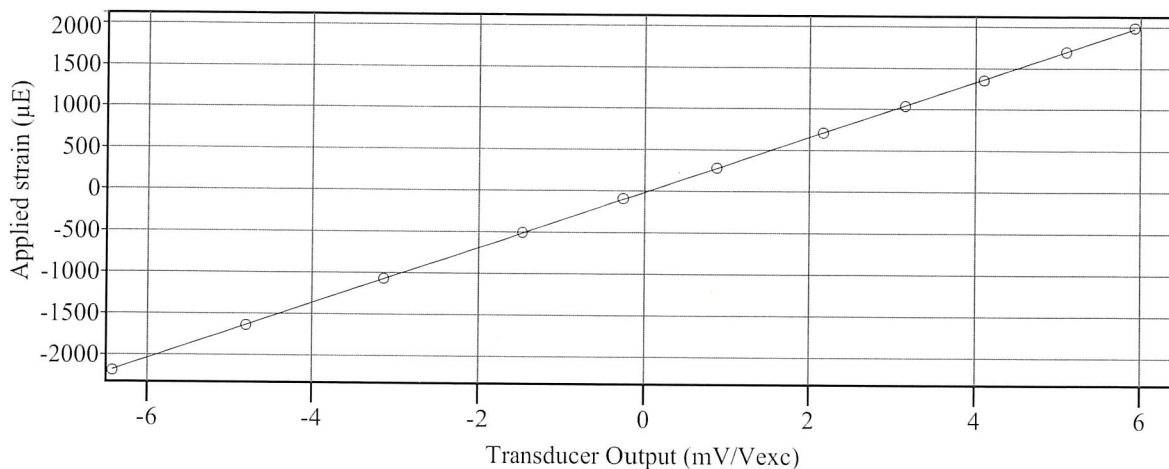

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

PDI Gage: 2759W

Calibration Date: _____

Calibration valid 2 years

Signature: _____

AUG 27 2026

