


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

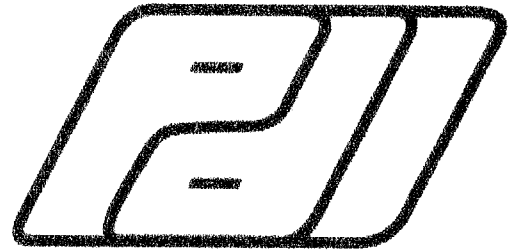

Serial No: 50796 Temperature: 19.6 °C

Model: PE Humidity: 55%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

985.9 g's/volt

R²: 0.999977 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 13Aug2026

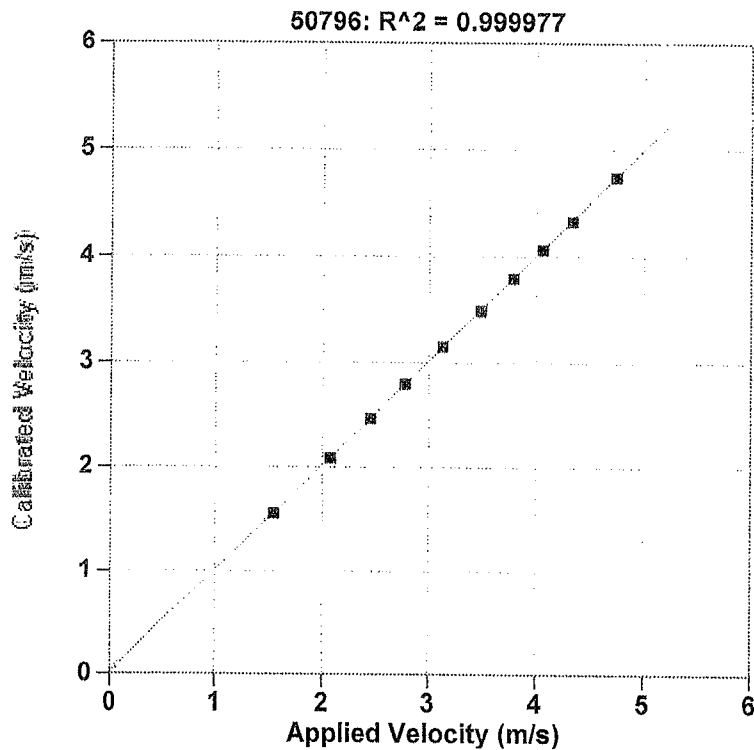

Reference Velocity	S/N 50796 Velocity
m/s	m/s
1.544	1.545
2.075	2.077
2.452	2.452
2.776	2.781
3.129	3.139
3.481	3.474
3.785	3.786
4.058	4.060
4.330	4.326
4.742	4.737
Maximum Acceleration: 1039 g's	