


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

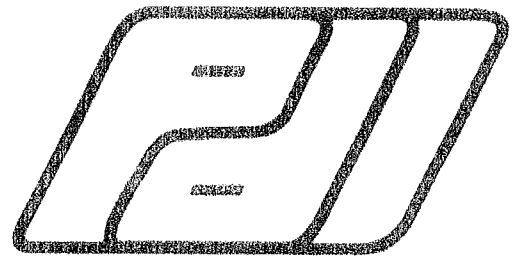

Serial No: 59172 Temperature: 23.1 °C

Model: PE Humidity: 40%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

977.1 g's/volt

R²: 0.999984 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 31Jul2026

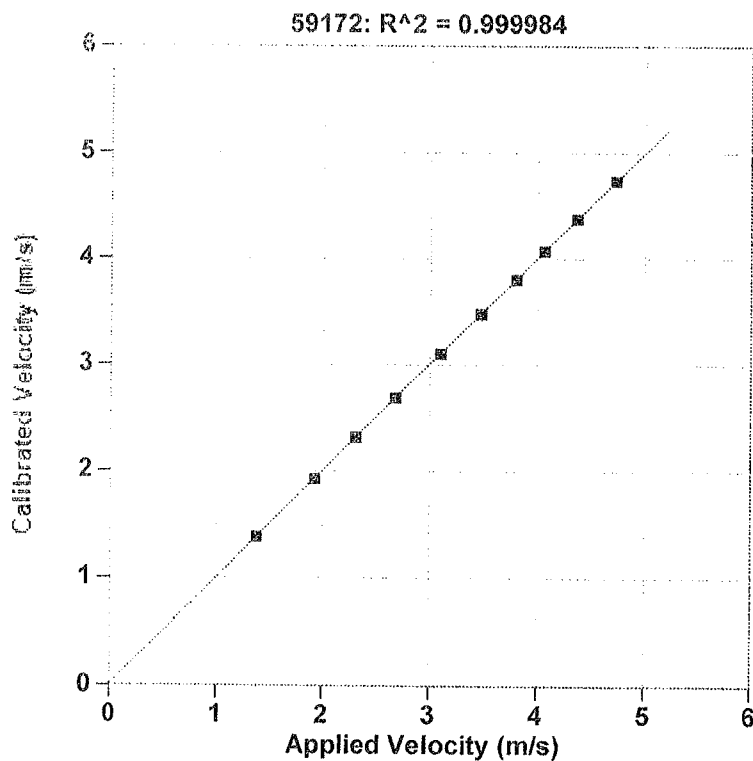

Reference Velocity	S/N 59172 Velocity
m/s	m/s
1.379	1.377
1.932	1.921
2.313	2.311
2.689	2.684
3.097	3.099
3.477	3.476
3.799	3.800
4.067	4.068
4.371	4.376
4.734	4.737

Maximum Acceleration: 1041 g's