


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

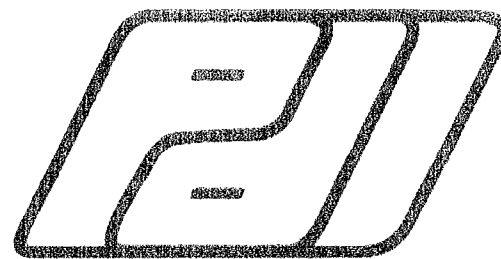

Serial No: 60505 Temperature: 23.1 °C

Model: PE Humidity: 40%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

971.9 g's/volt

R²: 0.999987 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson


William Johnson

Signed

Calibration valid 2 years

From: 31Jul2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

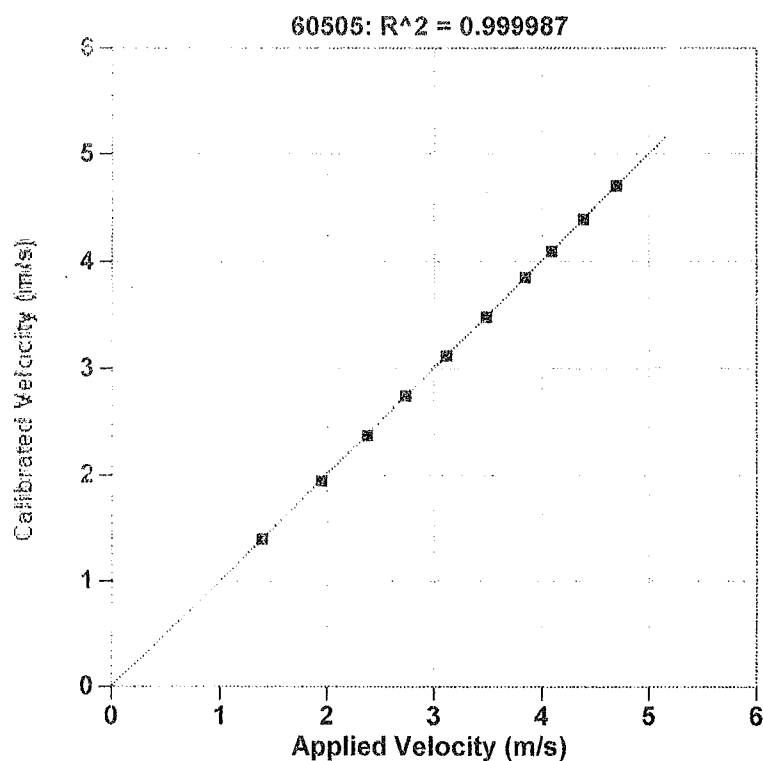

Reference Velocity	S/N 60505 Velocity
m/s	m/s
1.393	1.397
1.947	1.940
2.375	2.370
2.740	2.745
3.113	3.116
3.479	3.481
3.848	3.849
4.092	4.088
4.389	4.390
4.702	4.703
Maximum Acceleration: 1031 g's	