


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

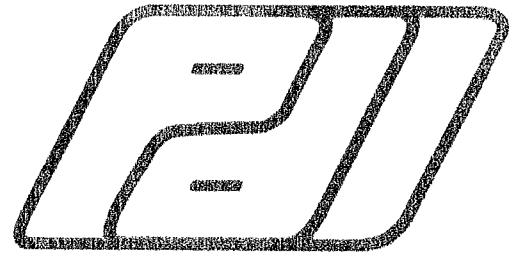

Serial No: 63546 Temperature: 23.1 °C

Model: PE Humidity: 40%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1044.3 g's/volt

R²: 0.999977 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 31Jul2026

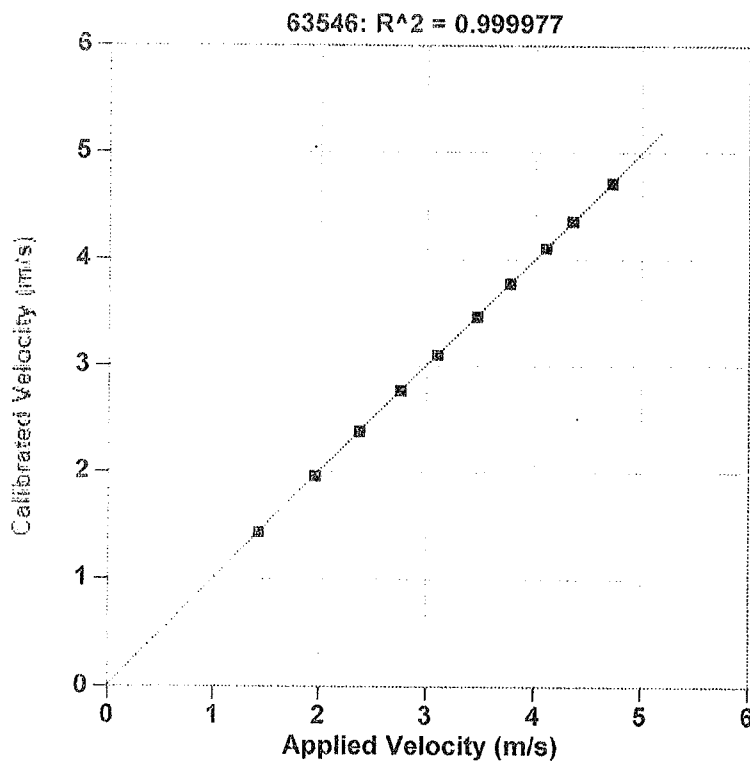

Reference Velocity	S/N 63546 Velocity
m/s	m/s
1.432	1.427
1.964	1.956
2.379	2.372
2.755	2.757
3.099	3.097
3.464	3.462
3.773	3.772
4.103	4.106
4.350	4.359
4.718	4.718
Maximum Acceleration: 1033 g's	